

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
 Data File : VU049125.D
 Acq On : 14 Jun 2022 19:43
 Operator : SY/MD
 Sample : N3278-15 10X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BF6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU049125.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	89	rBV	80956	89652	12.12%	1.740%
2	1.913	170	178	188	rBV	57369	74042	10.01%	1.437%
3	2.565	370	381	397	rVB	119861	195369	26.40%	3.793%
4	2.826	444	462	463	rBV	7747	16480	2.23%	0.320%
5	3.044	519	530	546	rVB4	9035	20983	2.84%	0.407%
6	3.189	560	575	590	rVB2	18154	43042	5.82%	0.836%
7	4.639	1010	1026	1074	rBV4	117849	455552	61.56%	8.844%
8	5.064	1143	1158	1177	rBV	103030	227141	30.70%	4.410%
9	5.726	1343	1364	1390	rBV2	215665	562484	76.01%	10.920%
10	6.250	1511	1527	1544	rBV	177259	340182	45.97%	6.604%
11	6.543	1605	1618	1630	rBV4	15542	31455	4.25%	0.611%
12	6.690	1649	1664	1685	rBV	134960	272671	36.85%	5.293%
13	7.565	1922	1936	1953	rBV2	76936	140403	18.97%	2.726%
14	7.899	2025	2040	2055	rBV	263325	463619	62.65%	9.000%
15	8.179	2114	2127	2140	rBV2	47950	84958	11.48%	1.649%
16	8.552	2233	2243	2256	rVB3	15086	25734	3.48%	0.500%
17	8.639	2256	2270	2307	rBV3	315758	739971	100.00%	14.365%
18	9.417	2500	2512	2536	rBV	232981	395360	53.43%	7.675%
19	10.758	2913	2929	2947	rBV	105630	175281	23.69%	3.403%
20	11.812	3246	3257	3275	rBV	243406	395765	53.48%	7.683%
21	12.192	3364	3375	3398	rBV	241617	401010	54.19%	7.785%




Sum of corrected areas: 5151154

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049125.D
Acq On : 14 Jun 2022 19:43
Operator : SY/MD
Sample : N3278-15 10X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BF6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

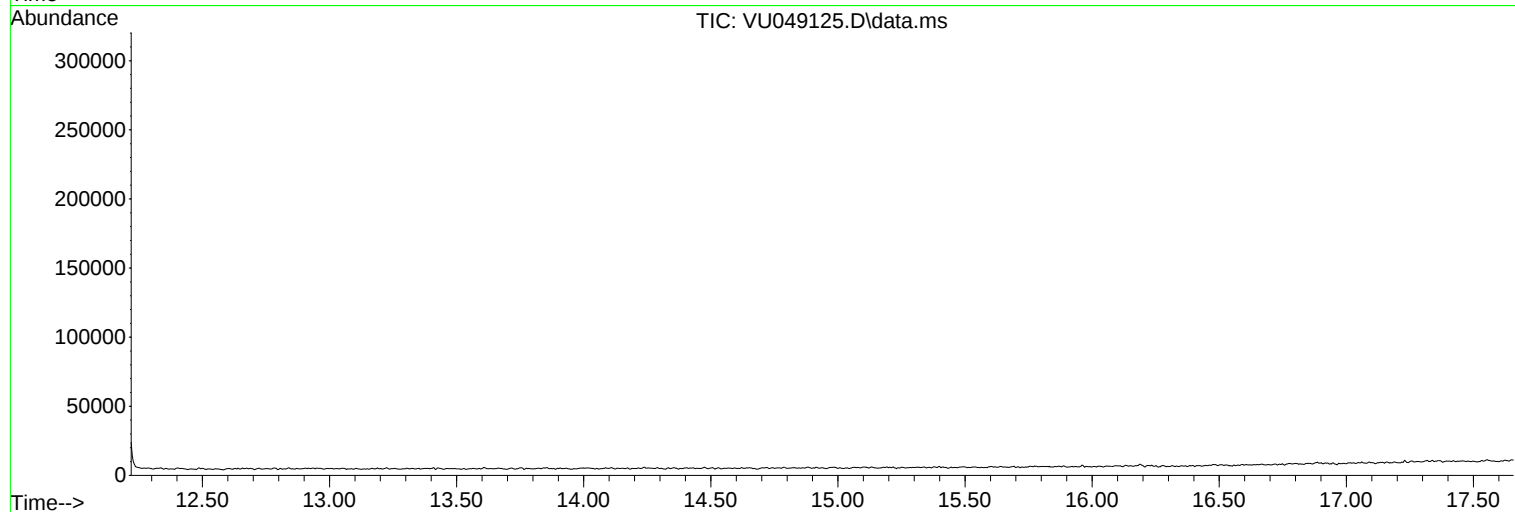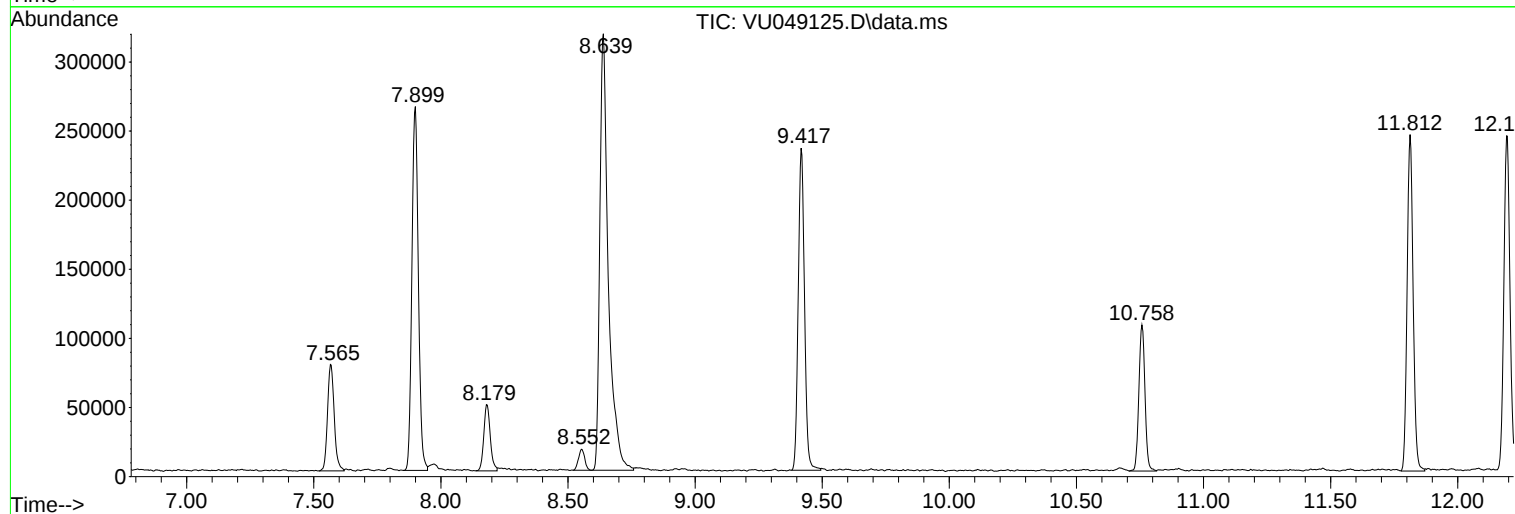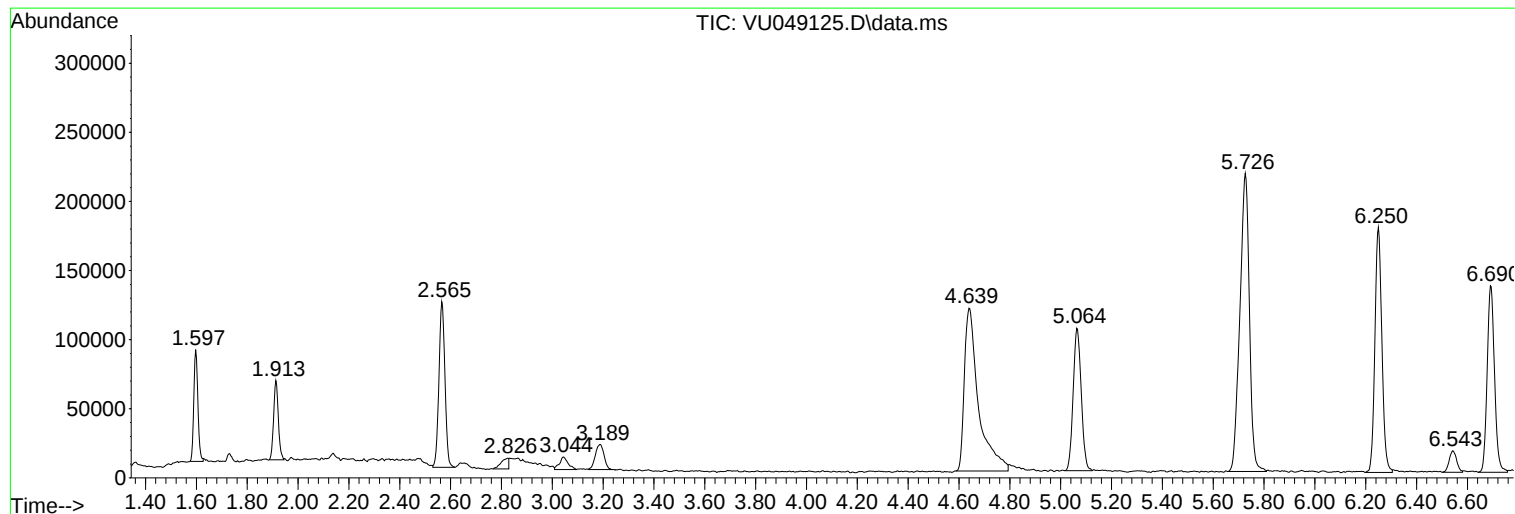

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049125.D
Acq On : 14 Jun 2022 19:43
Operator : SY/MD
Sample : N3278-15 10X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BF6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049125.D
Acq On : 14 Jun 2022 19:43
Operator : SY/MD
Sample : N3278-15 10X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BF6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc