

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
 Data File : VU049134.D
 Acq On : 14 Jun 2022 23:41
 Operator : SY/MD
 Sample : VU0614WBL02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK086

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.1 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU049135.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	95	rBV	87681	98775	13.35%	1.979%
2	1.912	171	178	191	rVB	61217	79041	10.69%	1.584%
3	2.568	370	382	398	rVB	123780	201924	27.30%	4.047%
4	3.047	520	531	542	rVB4	6227	12314	1.66%	0.247%
5	4.636	1008	1025	1062	rBV	99609	335397	45.35%	6.721%
6	5.067	1140	1159	1180	rBV	103118	229854	31.08%	4.606%
7	5.726	1344	1364	1384	rBV2	218895	569294	76.97%	11.409%
8	6.250	1513	1527	1548	rBV	177169	340057	45.98%	6.815%
9	6.690	1651	1664	1685	rBV	136199	268801	36.34%	5.387%
10	7.565	1922	1936	1953	rBV	75183	139958	18.92%	2.805%
11	7.899	2027	2040	2056	rBV	274403	480034	64.90%	9.620%
12	7.970	2058	2062	2072	rVB3	5220	7678	1.04%	0.154%
13	8.182	2114	2128	2143	rBV2	47236	85065	11.50%	1.705%
14	8.636	2257	2269	2316	rBV2	345470	739649	100.00%	14.822%
15	9.417	2499	2512	2534	rBV	237251	407276	55.06%	8.162%
16	10.758	2916	2929	2941	rBV	108261	175507	23.73%	3.517%
17	11.812	3246	3257	3278	rBV	243217	398047	53.82%	7.977%
18	12.192	3363	3375	3392	rBV	243851	407297	55.07%	8.162%
19	14.095	3955	3967	3980	rBV2	7180	14080	1.90%	0.282%




Sum of corrected areas: 4990048

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049134.D
Acq On : 14 Jun 2022 23:41
Operator : SY/MD
Sample : VU0614WBL02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK086

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

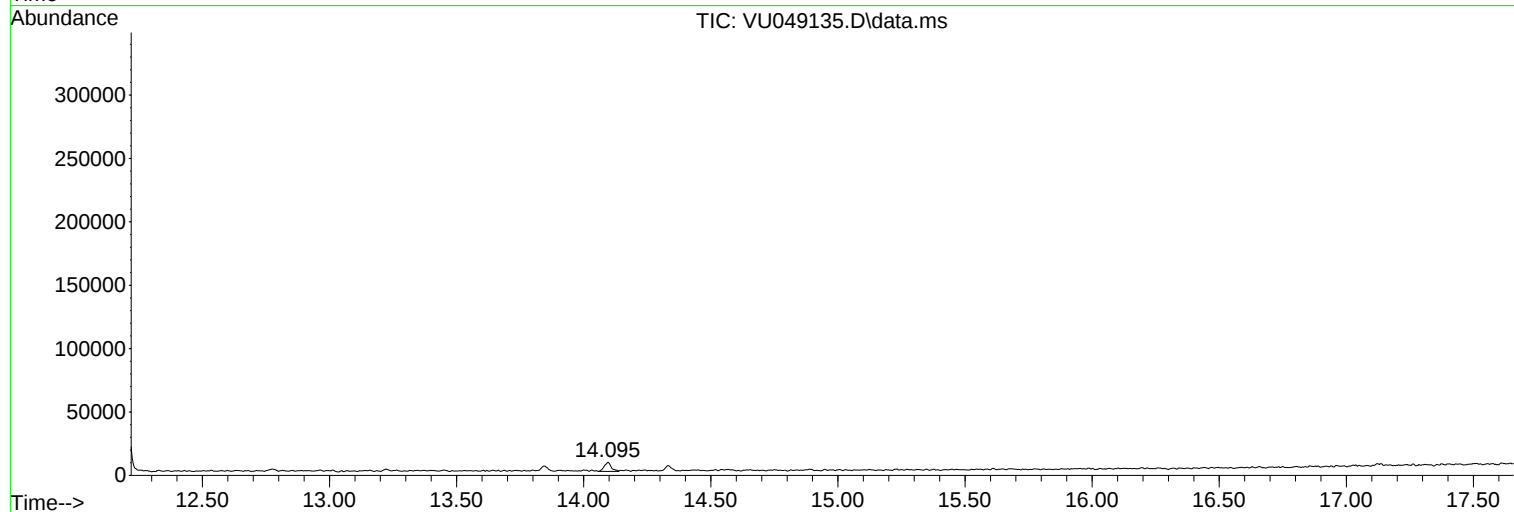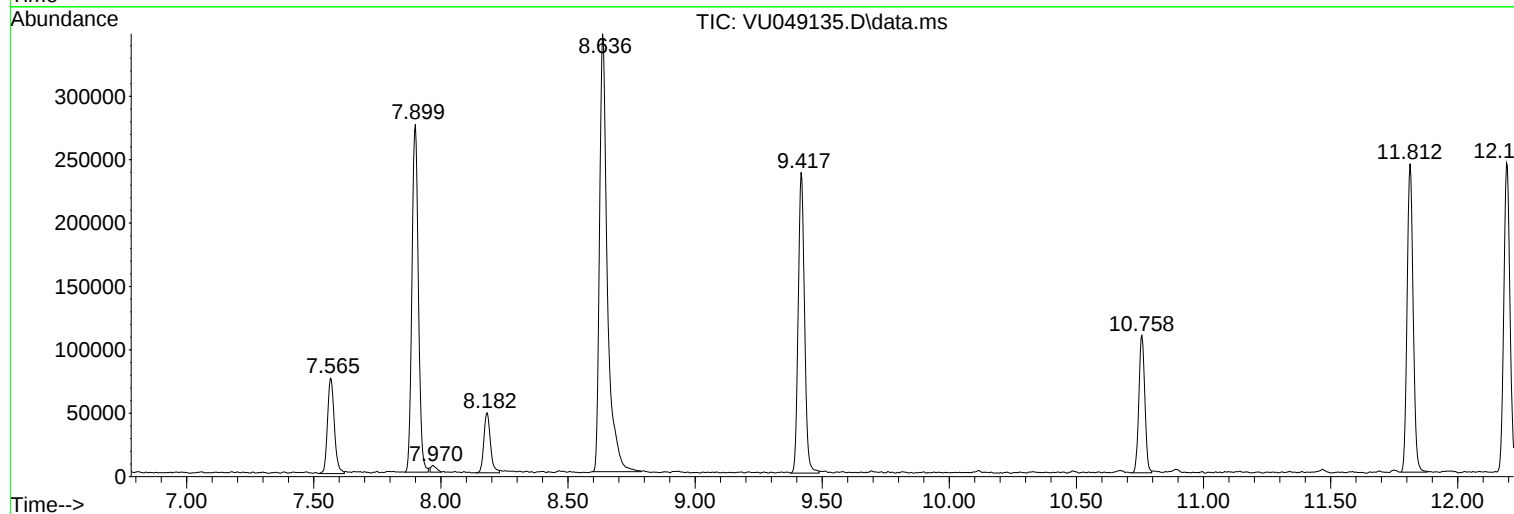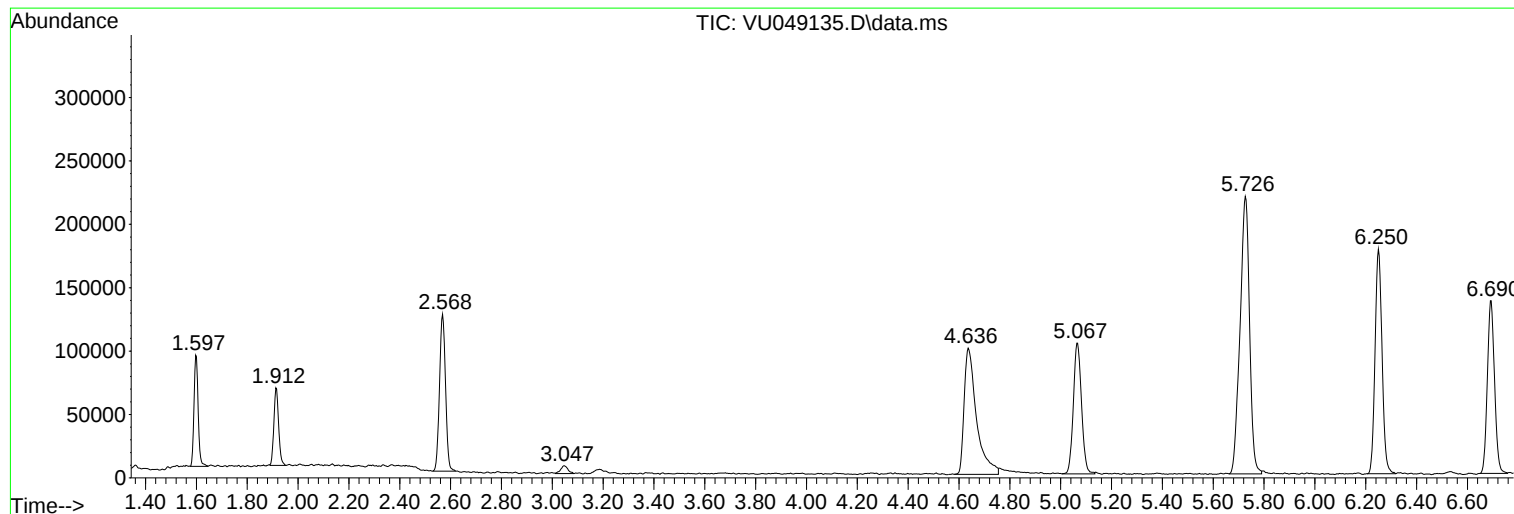

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049134.D
Acq On : 14 Jun 2022 23:41
Operator : SY/MD
Sample : VU0614WBL02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK086

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049134.D
Acq On : 14 Jun 2022 23:41
Operator : SY/MD
Sample : VU0614WBL02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK086

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------