

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
 Data File : VU049135.D
 Acq On : 15 Jun 2022 00:05
 Operator : SY/MD
 Sample : N3274-01 250X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B91

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU049135.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	70	80	94	rBV	78862	92750	12.29%	1.850%
2	1.912	170	178	188	rBV	57882	72790	9.65%	1.452%
3	2.568	369	382	397	rBV	111903	183773	24.36%	3.666%
4	3.047	520	531	544	rVB3	8665	16746	2.22%	0.334%
5	3.186	563	574	587	rBV	15499	34060	4.51%	0.679%
6	4.639	1008	1026	1057	rBV3	128390	441977	58.58%	8.817%
7	5.063	1141	1158	1178	rBV	100795	226038	29.96%	4.509%
8	5.726	1344	1364	1392	rBV2	210591	556266	73.72%	11.097%
9	6.250	1511	1527	1549	rBV	175016	337463	44.73%	6.732%
10	6.693	1649	1665	1682	rBV	134170	265564	35.20%	5.298%
11	7.568	1925	1937	1950	rBV2	75247	130989	17.36%	2.613%
12	7.899	2025	2040	2057	rBV	258366	452144	59.92%	9.020%
13	7.970	2057	2062	2072	rVB5	5059	8081	1.07%	0.161%
14	8.182	2116	2128	2140	rBV2	46200	80931	10.73%	1.615%
15	8.636	2257	2269	2308	rBV2	345150	754519	100.00%	15.052%
16	9.417	2497	2512	2535	rBV	231802	400031	53.02%	7.980%
17	10.758	2916	2929	2942	rBV	108620	176647	23.41%	3.524%
18	11.812	3244	3257	3273	rBV	236533	385094	51.04%	7.682%
19	12.195	3358	3376	3393	rBV	238407	396890	52.60%	7.918%




Sum of corrected areas: 5012753

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049135.D
Acq On : 15 Jun 2022 00:05
Operator : SY/MD
Sample : N3274-01 250X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B91

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

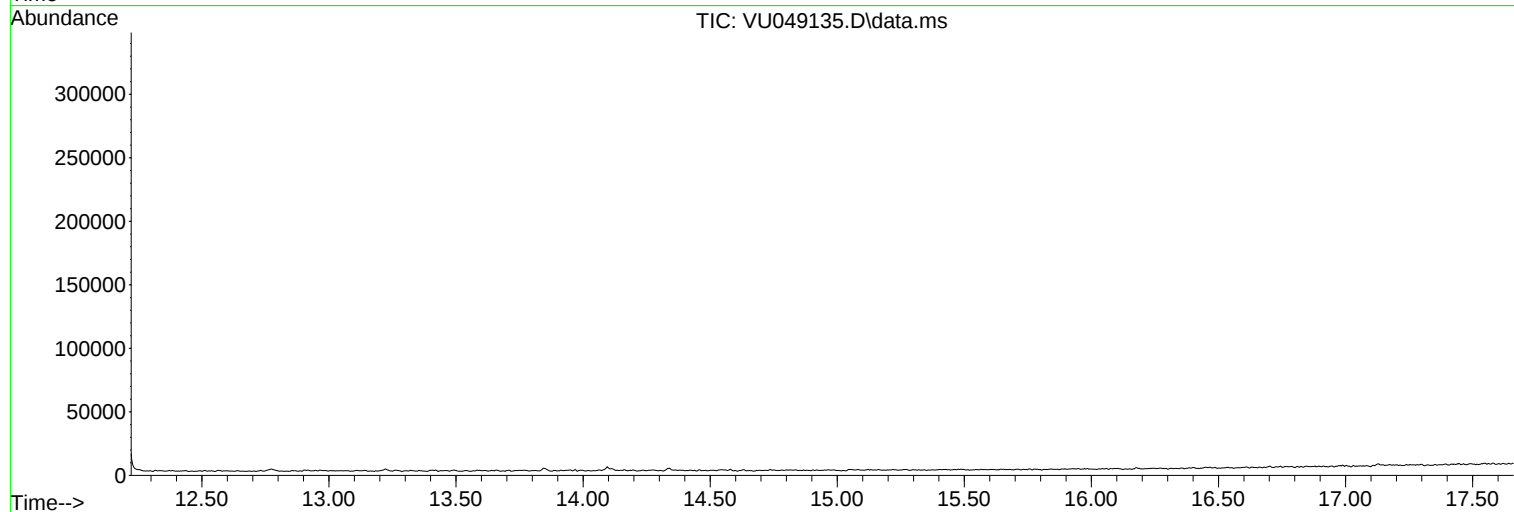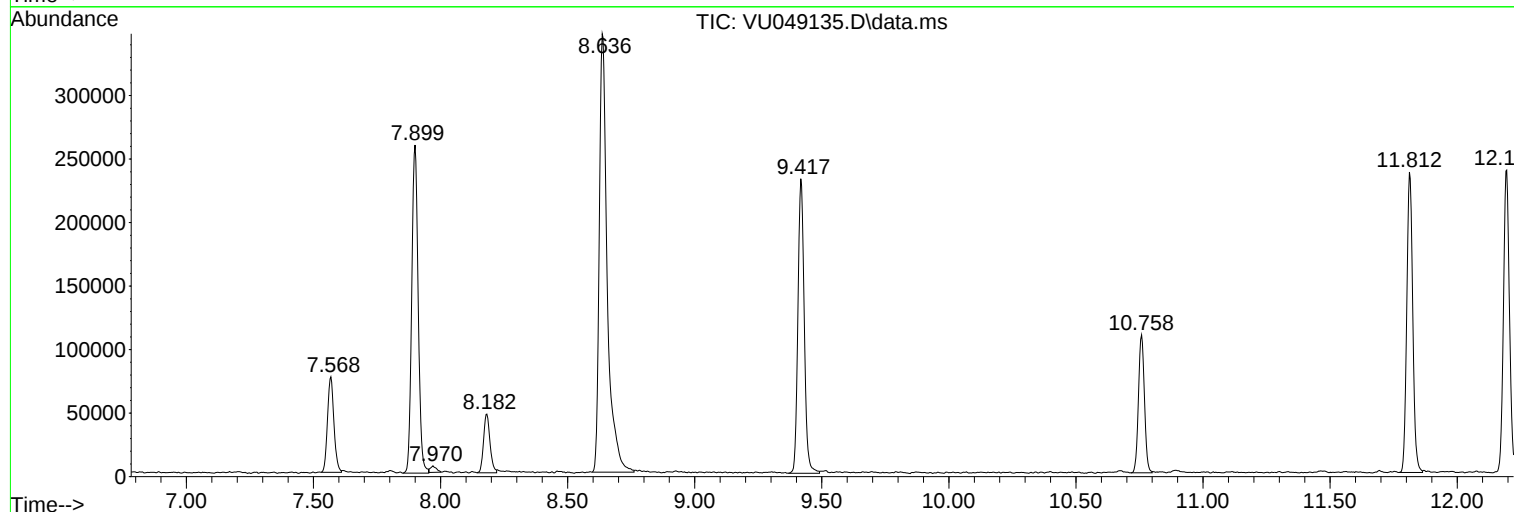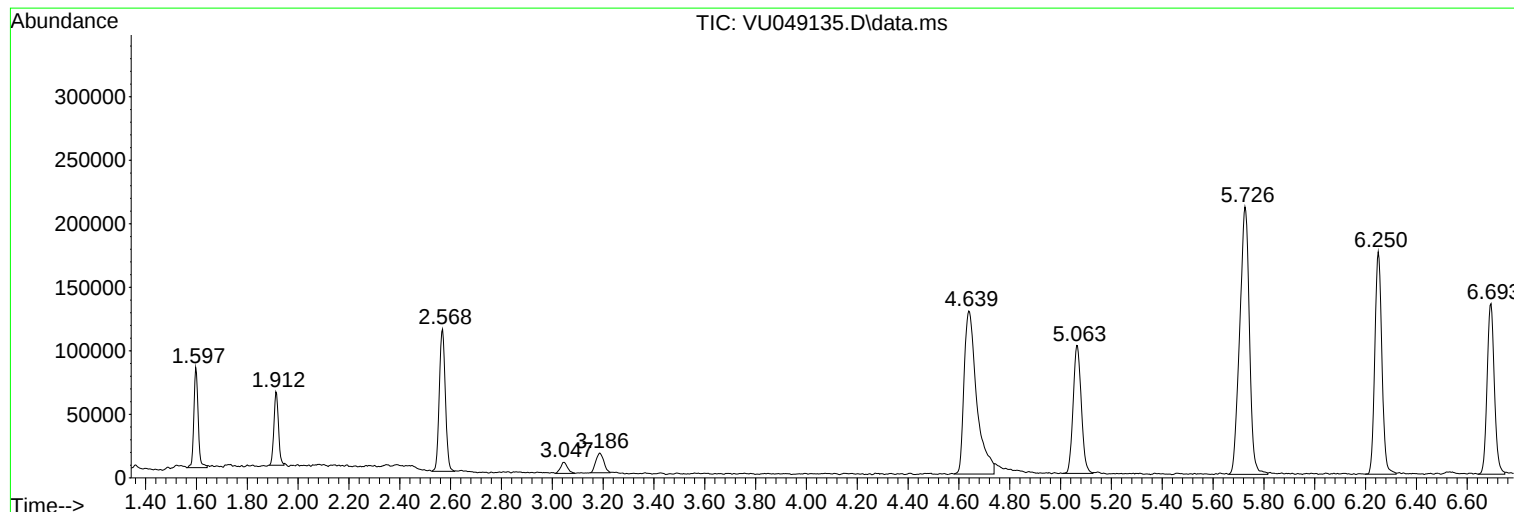

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049135.D
Acq On : 15 Jun 2022 00:05
Operator : SY/MD
Sample : N3274-01 250X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B91

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049135.D
Acq On : 15 Jun 2022 00:05
Operator : SY/MD
Sample : N3274-01 250X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B91

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------