

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
 Data File : VU049139.D
 Acq On : 15 Jun 2022 01:40
 Operator : SY/MD
 Sample : N3274-05 250X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B95

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU049139.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	93	rBV	79189	89599	4.41%	1.240%
2	1.912	171	178	191	rVB	57305	73919	3.64%	1.023%
3	2.141	241	249	258	rBV	16339	22805	1.12%	0.316%
4	2.568	371	382	398	rVB	116008	187843	9.24%	2.600%
5	3.186	561	574	591	rBV2	17126	39363	1.94%	0.545%
6	4.639	1008	1026	1074	rBV2	125356	457496	22.50%	6.332%
7	5.063	1141	1158	1177	rBV2	102077	223921	11.01%	3.099%
8	5.726	1343	1364	1391	rBV2	211476	560701	27.58%	7.760%
9	6.250	1514	1527	1546	rBV	173233	329463	16.20%	4.560%
10	6.542	1599	1618	1648	rBV	1063416	2033179	100.00%	28.139%
11	6.690	1652	1664	1682	rVB	134461	266173	13.09%	3.684%
12	7.568	1924	1937	1954	rBV	74607	137548	6.77%	1.904%
13	7.899	2024	2040	2057	rBV	264850	463973	22.82%	6.421%
14	8.179	2116	2127	2144	rBV	45988	80593	3.96%	1.115%
15	8.552	2231	2243	2257	rBV2	86714	147036	7.23%	2.035%
16	8.635	2257	2269	2300	rBV2	346079	751161	36.95%	10.396%
17	9.417	2498	2512	2537	rBV	232682	390175	19.19%	5.400%
18	10.758	2917	2929	2945	rBV2	107276	176089	8.66%	2.437%
19	11.812	3245	3257	3275	rBV	235952	388097	19.09%	5.371%
20	12.195	3364	3376	3394	rBV	246917	406271	19.98%	5.623%




Sum of corrected areas: 7225405

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049139.D
Acq On : 15 Jun 2022 01:40
Operator : SY/MD
Sample : N3274-05 250X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B95

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

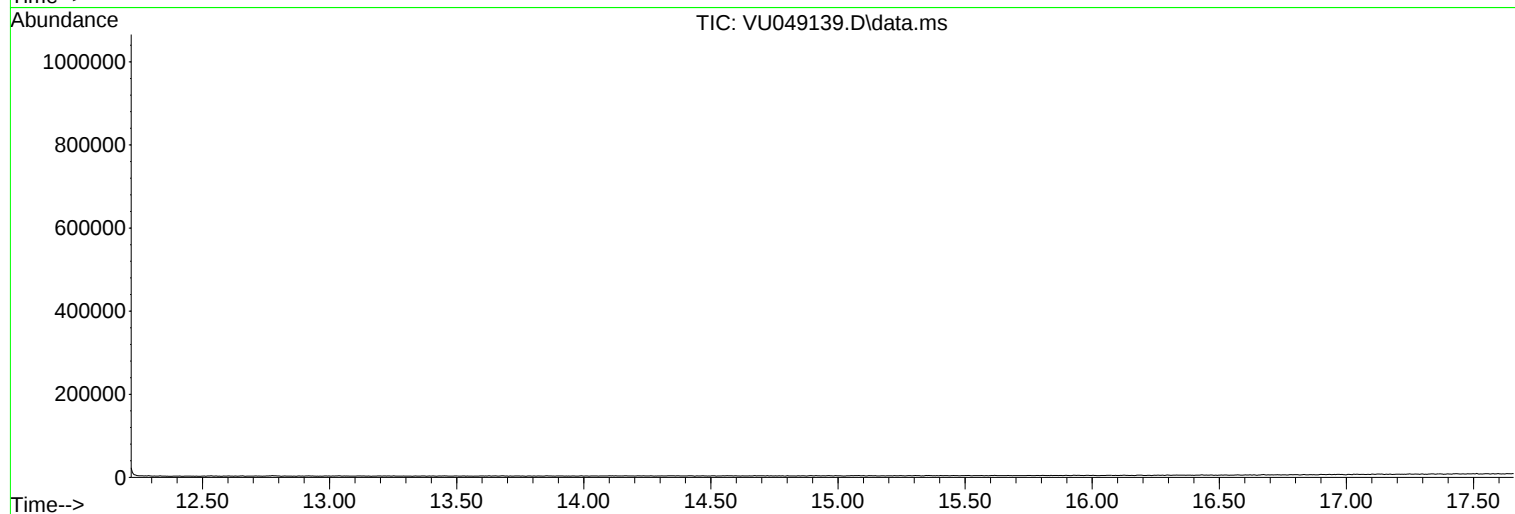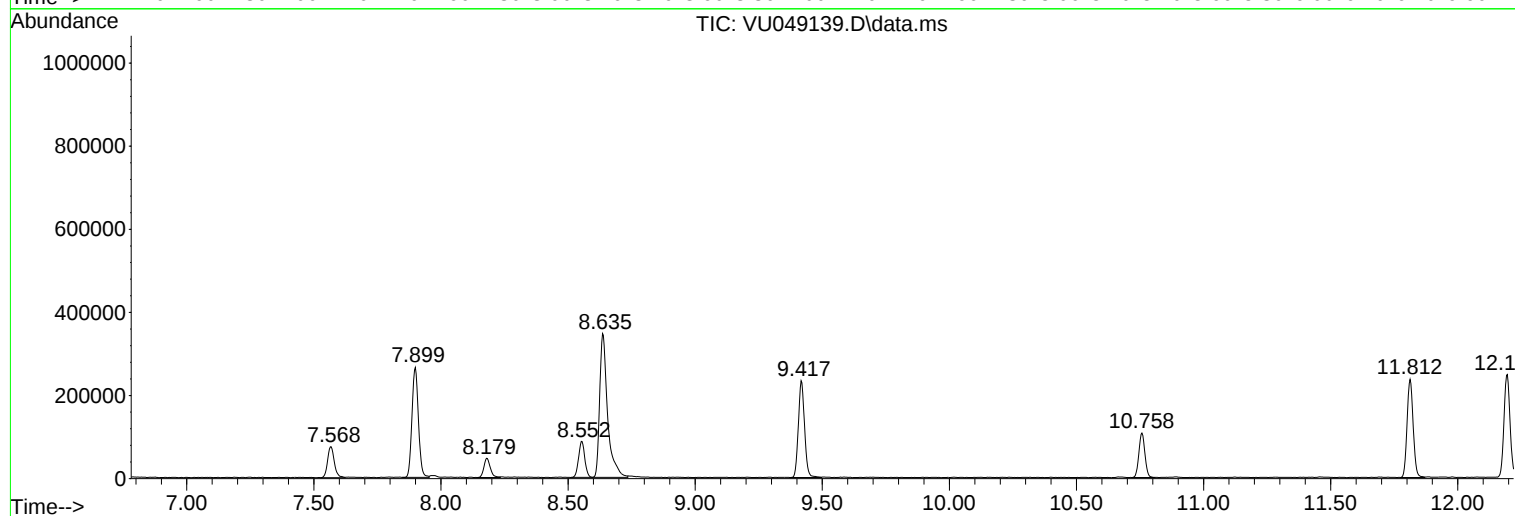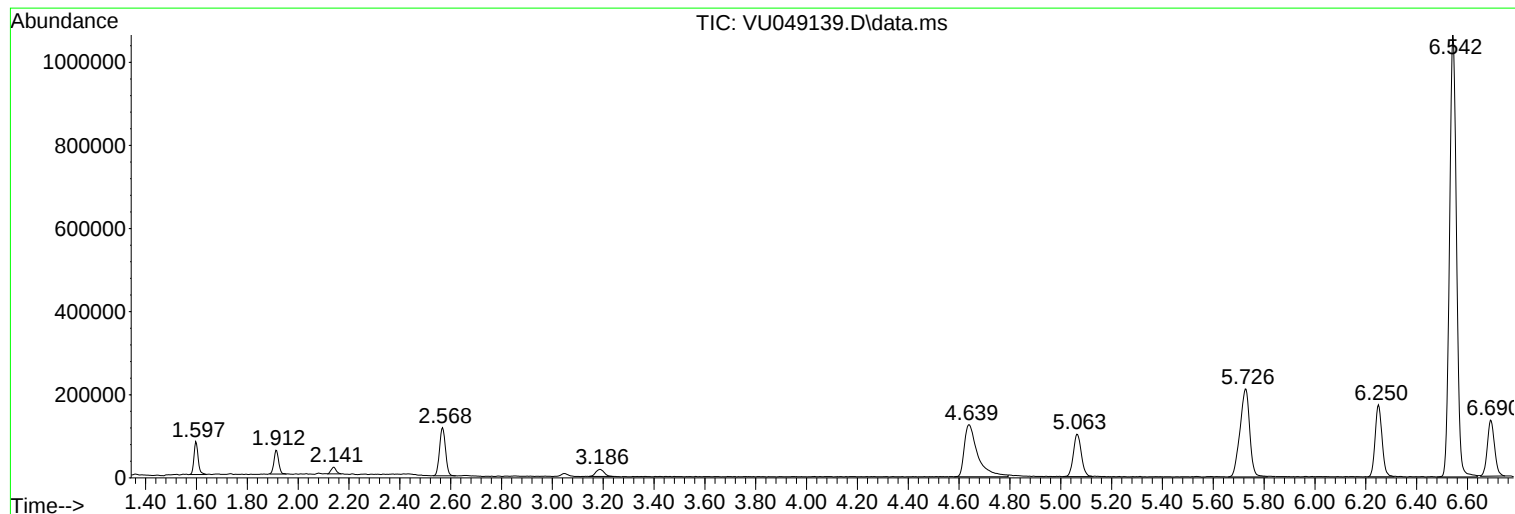

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049139.D
Acq On : 15 Jun 2022 01:40
Operator : SY/MD
Sample : N3274-05 250X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B95

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049139.D
Acq On : 15 Jun 2022 01:40
Operator : SY/MD
Sample : N3274-05 250X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B95

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------