

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
 Data File : VU049140.D
 Acq On : 15 Jun 2022 02:04
 Operator : SY/MD
 Sample : N3274-06 250X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B96

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU049140.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	91	rBV	78391	87370	11.72%	1.709%
2	1.913	171	178	187	rBV	57216	70935	9.52%	1.388%
3	2.568	370	382	397	rBV	114509	187052	25.10%	3.660%
4	3.048	522	531	542	rVB2	8243	15316	2.05%	0.300%
5	3.189	558	575	588	rBV	19894	47808	6.41%	0.935%
6	4.639	1007	1026	1072	rBV3	133780	493175	66.17%	9.649%
7	5.064	1143	1158	1181	rBV2	99434	226063	30.33%	4.423%
8	5.726	1343	1364	1382	rBV2	210184	550760	73.90%	10.776%
9	6.250	1514	1527	1556	rVB	173782	330476	44.34%	6.466%
10	6.543	1607	1618	1628	rBV5	23465	44777	6.01%	0.876%
11	6.694	1650	1665	1682	rBV	132347	265643	35.64%	5.198%
12	7.565	1924	1936	1958	rBV	70847	130663	17.53%	2.557%
13	7.899	2023	2040	2056	rBV	263077	460978	61.85%	9.019%
14	8.182	2116	2128	2143	rBV	45668	79792	10.71%	1.561%
15	8.555	2235	2244	2254	rVB2	15417	24716	3.32%	0.484%
16	8.639	2254	2270	2300	rBV2	338113	745324	100.00%	14.583%
17	9.417	2499	2512	2529	rBV	231056	388386	52.11%	7.599%
18	10.758	2917	2929	2945	rBV	106338	173971	23.34%	3.404%
19	11.812	3245	3257	3281	rBV	241733	387910	52.05%	7.590%
20	12.192	3363	3375	3393	rBV	241128	399858	53.65%	7.824%




Sum of corrected areas: 5110973

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049140.D
Acq On : 15 Jun 2022 02:04
Operator : SY/MD
Sample : N3274-06 250X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B96

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

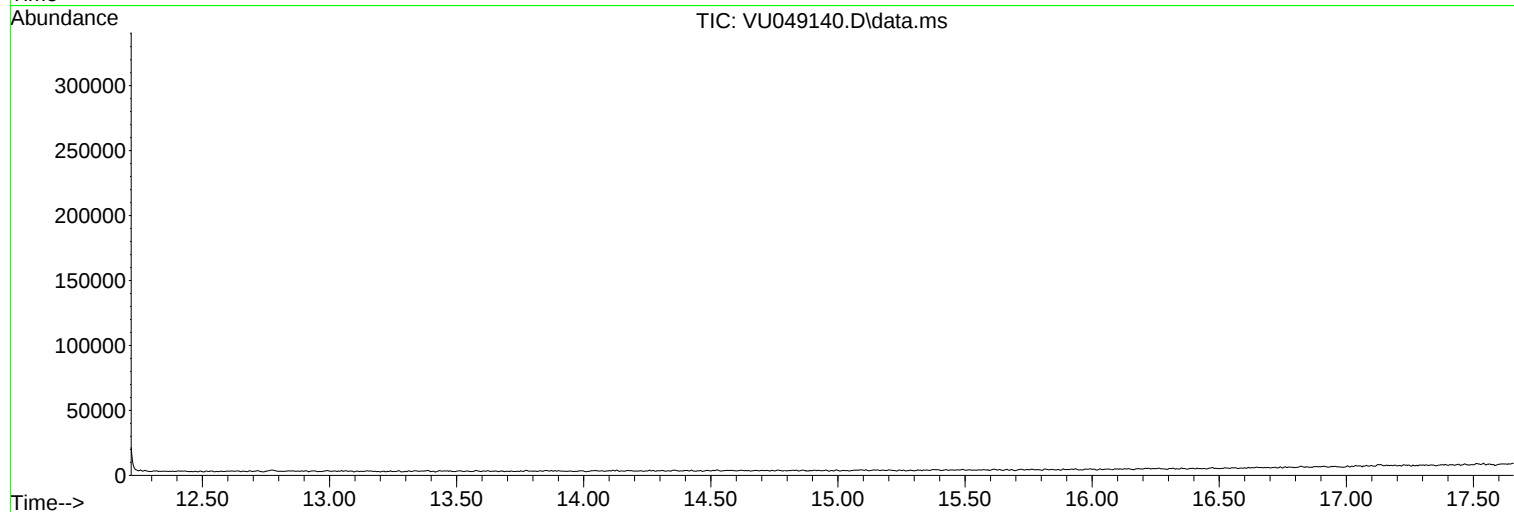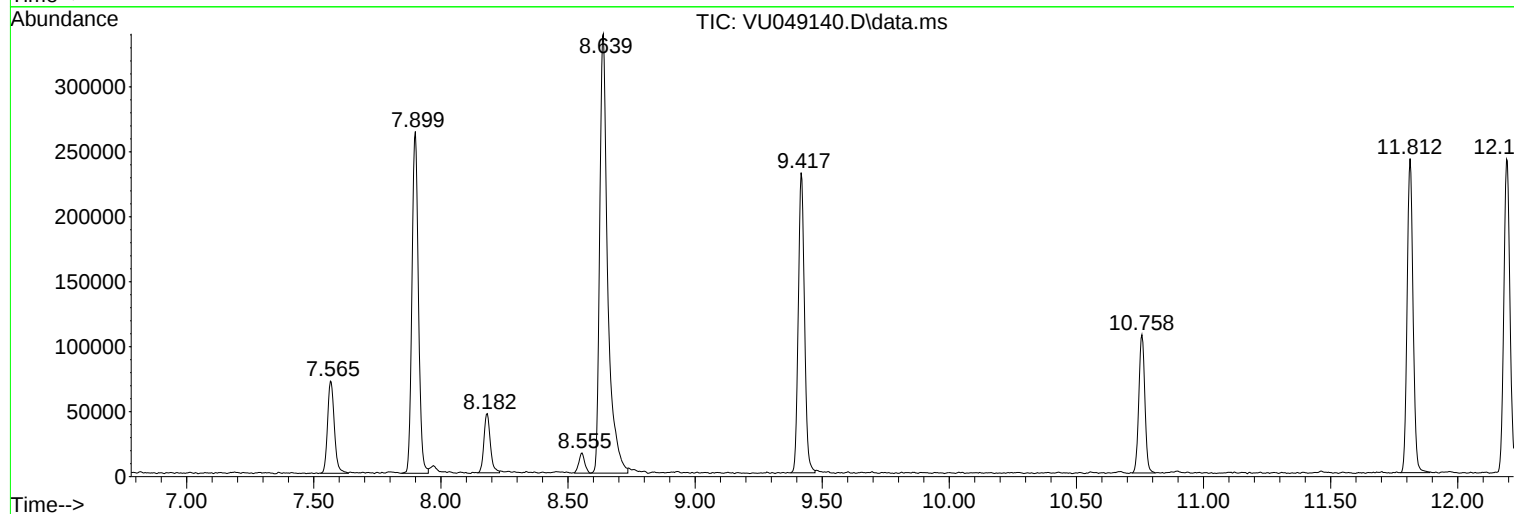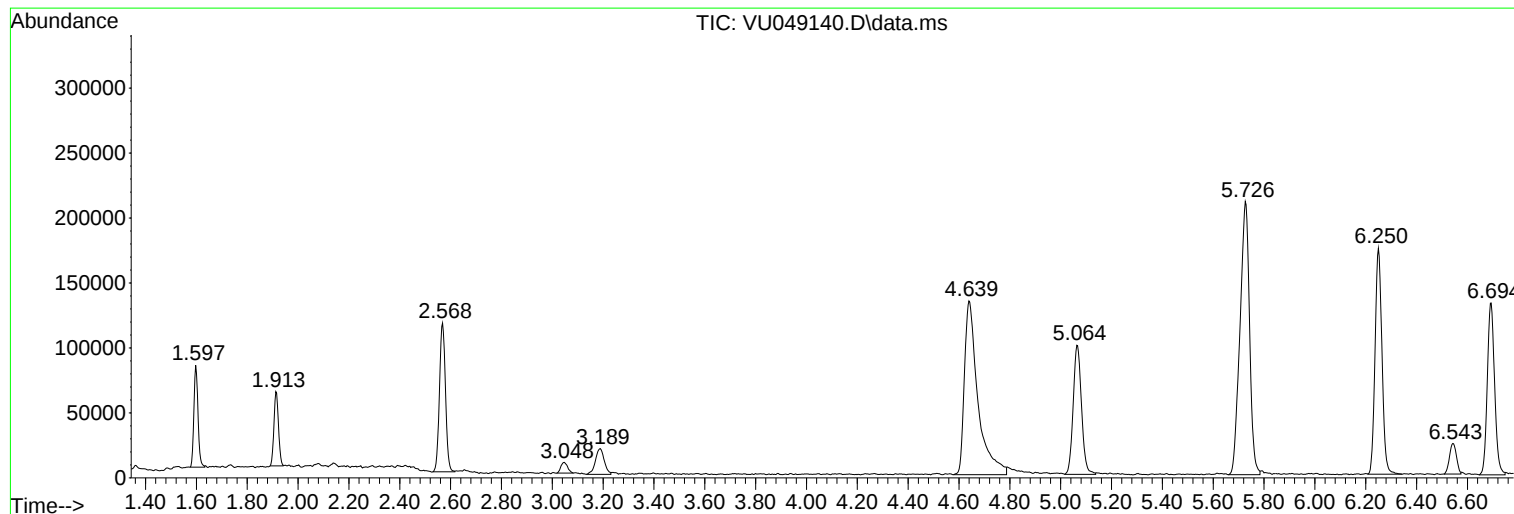

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049140.D
Acq On : 15 Jun 2022 02:04
Operator : SY/MD
Sample : N3274-06 250X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B96

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049140.D
Acq On : 15 Jun 2022 02:04
Operator : SY/MD
Sample : N3274-06 250X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B96

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc