

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
 Data File : VU049141.D
 Acq On : 15 Jun 2022 02:28
 Operator : SY/MD
 Sample : N3274-07 250X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B97

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU049141.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	90	rVB	75954	84692	11.12%	1.647%
2	1.912	170	178	188	rBV	55858	71017	9.32%	1.381%
3	2.568	370	382	397	rVB	111509	181200	23.78%	3.523%
4	3.047	520	531	540	rBV3	8950	15713	2.06%	0.306%
5	3.186	559	574	592	rBV2	23103	53258	6.99%	1.036%
6	4.639	1004	1026	1069	rBV3	134322	501937	65.88%	9.760%
7	5.063	1139	1158	1179	rBV	99800	223765	29.37%	4.351%
8	5.726	1340	1364	1392	rBV2	209956	555191	72.87%	10.795%
9	6.250	1511	1527	1551	rBV	171795	328529	43.12%	6.388%
10	6.543	1603	1618	1634	rBV6	17050	34342	4.51%	0.668%
11	6.694	1647	1665	1691	rBV3	130980	267017	35.04%	5.192%
12	7.565	1922	1936	1958	rBV	71268	131313	17.23%	2.553%
13	7.899	2024	2040	2056	rBV	260662	461277	60.54%	8.969%
14	7.970	2056	2062	2073	rVB2	4601	9090	1.19%	0.177%
15	8.182	2117	2128	2147	rBV2	44252	79148	10.39%	1.539%
16	8.555	2234	2244	2255	rVB3	15817	25414	3.34%	0.494%
17	8.636	2255	2269	2305	rBV2	344173	761939	100.00%	14.815%
18	9.417	2497	2512	2532	rBV	231274	392640	51.53%	7.635%
19	10.758	2917	2929	2944	rBV	110246	177199	23.26%	3.445%
20	11.812	3243	3257	3273	rBV	241607	387376	50.84%	7.532%
21	12.192	3362	3375	3394	rBV	241530	400884	52.61%	7.795%




Sum of corrected areas: 5142941

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049141.D
Acq On : 15 Jun 2022 02:28
Operator : SY/MD
Sample : N3274-07 250X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B97

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

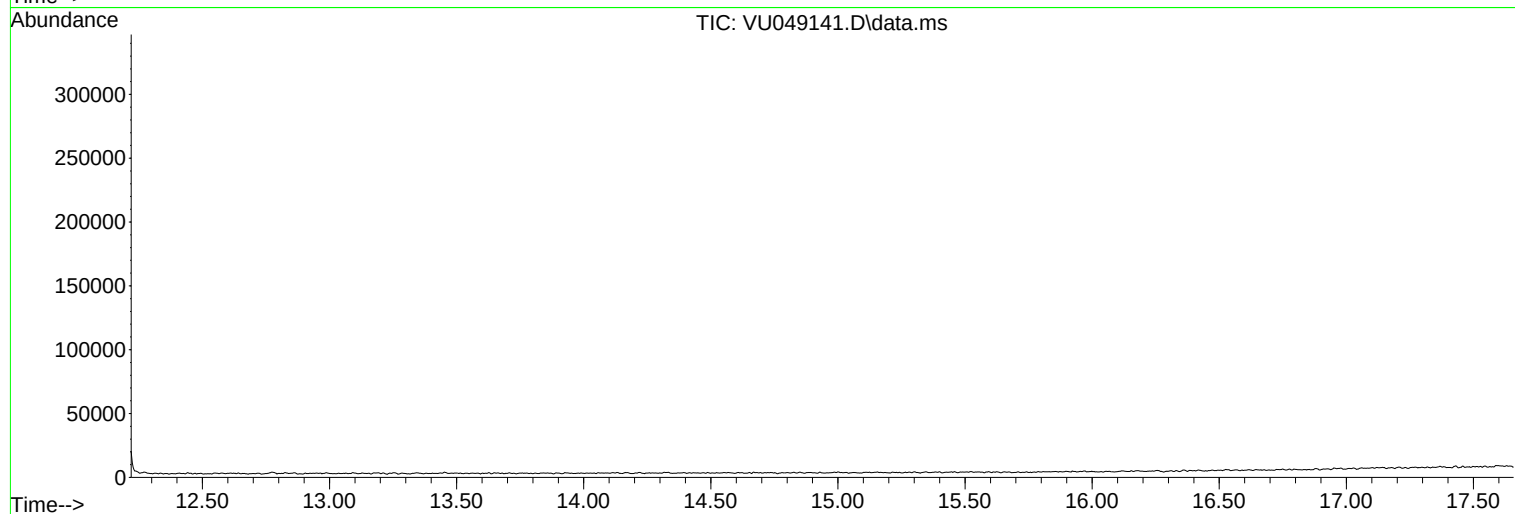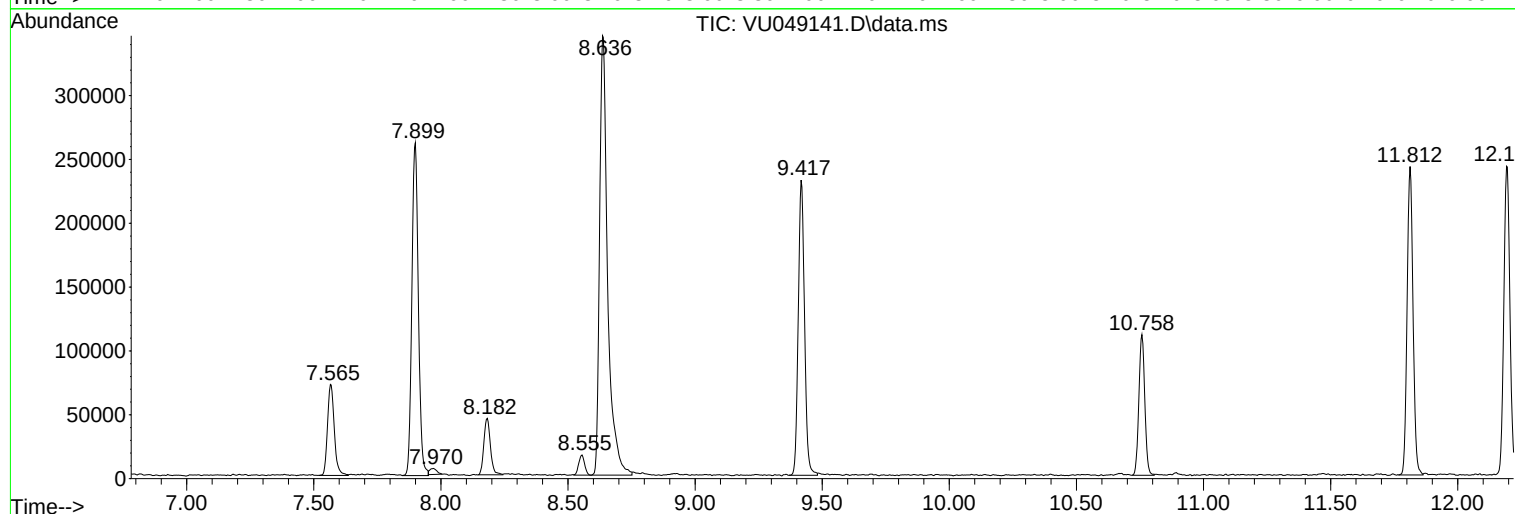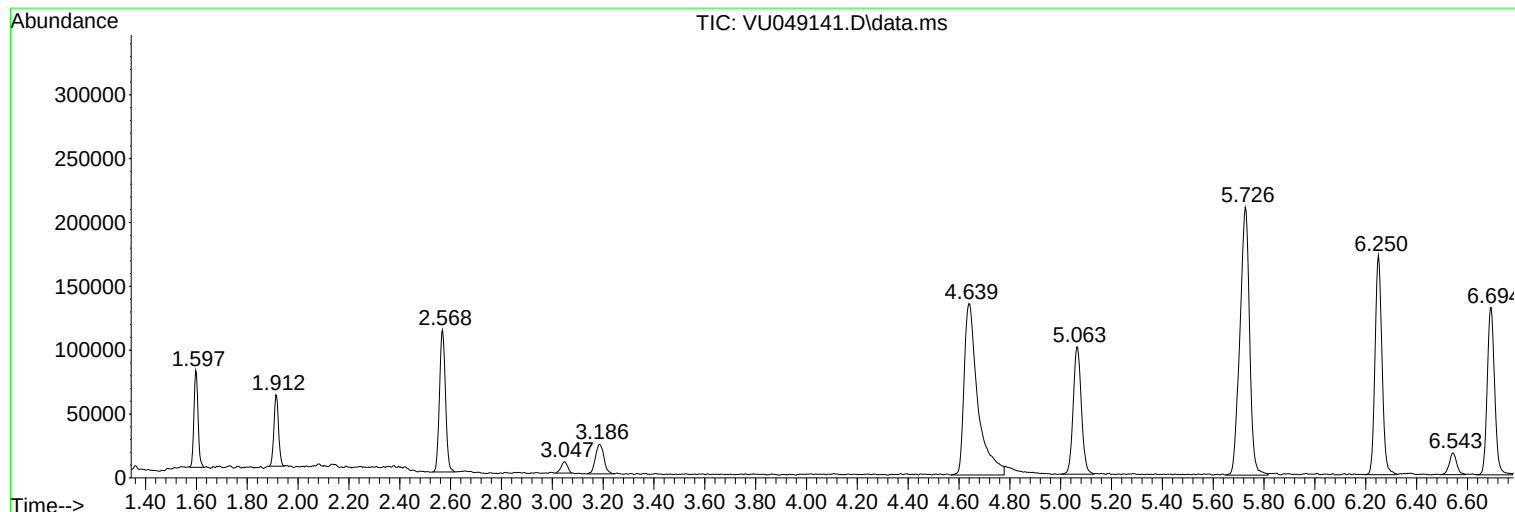

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049141.D
Acq On : 15 Jun 2022 02:28
Operator : SY/MD
Sample : N3274-07 250X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B97

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049141.D
Acq On : 15 Jun 2022 02:28
Operator : SY/MD
Sample : N3274-07 250X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B97

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc