

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
 Data File : VU049144.D
 Acq On : 15 Jun 2022 03:39
 Operator : SY/MD
 Sample : N3274-10 250X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BA0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU049144.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	90	rBV	77480	87730	11.89%	1.752%
2	1.916	171	179	189	rBV	54891	69169	9.37%	1.381%
3	2.568	371	382	396	rBV	112447	181954	24.65%	3.634%
4	3.047	522	531	544	rVB2	9787	17685	2.40%	0.353%
5	3.186	558	574	595	rVB	21006	50078	6.78%	1.000%
6	4.639	1011	1026	1060	rBV3	128979	465931	63.12%	9.305%
7	5.067	1142	1159	1180	rBV	96858	213891	28.98%	4.272%
8	5.726	1341	1364	1390	rBV2	209354	544442	73.76%	10.873%
9	6.250	1511	1527	1549	rBV	174844	339537	46.00%	6.781%
10	6.542	1604	1618	1630	rVB7	9833	18858	2.55%	0.377%
11	6.690	1651	1664	1681	rBV	131556	259879	35.21%	5.190%
12	7.565	1923	1936	1953	rBV	69088	126007	17.07%	2.516%
13	7.899	2026	2040	2054	rBV	253612	445155	60.31%	8.890%
14	8.182	2114	2128	2143	rBV	43782	78647	10.66%	1.571%
15	8.552	2231	2243	2253	rBV6	7443	13189	1.79%	0.263%
16	8.639	2253	2270	2311	rBV2	334069	738110	100.00%	14.741%
17	9.417	2497	2512	2532	rBV	232118	394815	53.49%	7.885%
18	10.758	2917	2929	2941	rBV	105563	170582	23.11%	3.407%
19	11.812	3243	3257	3273	rBV	246730	397440	53.85%	7.937%
20	12.192	3361	3375	3392	rBV	239248	394137	53.40%	7.871%




Sum of corrected areas: 5007236

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049144.D
Acq On : 15 Jun 2022 03:39
Operator : SY/MD
Sample : N3274-10 250X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BA0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

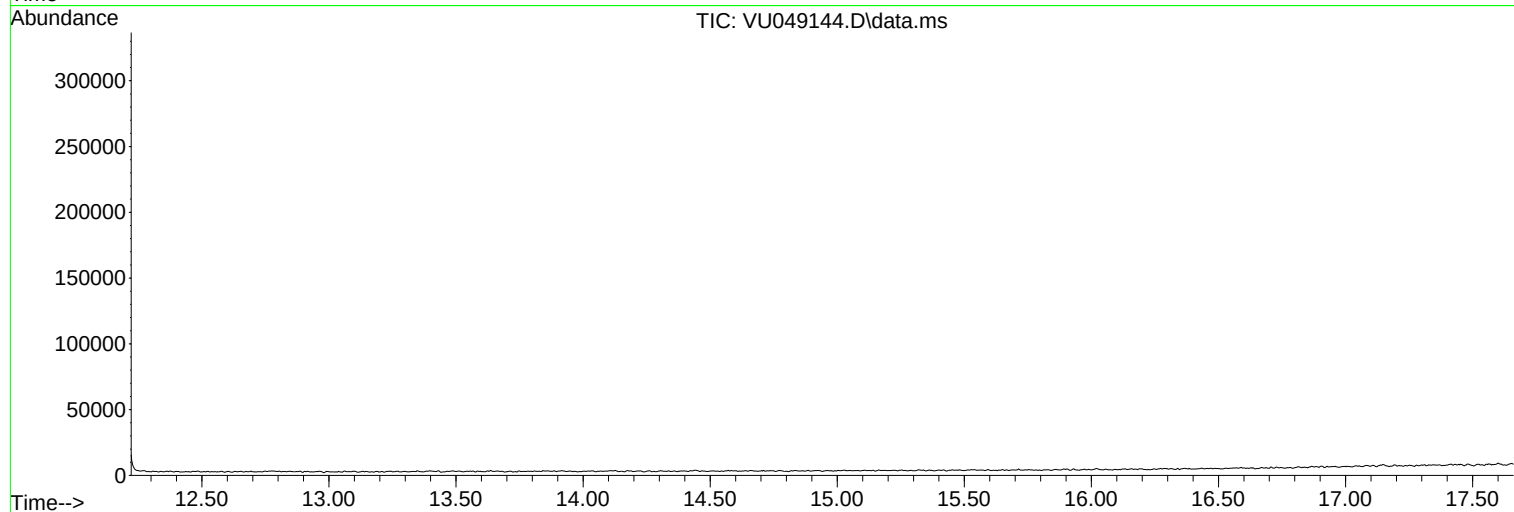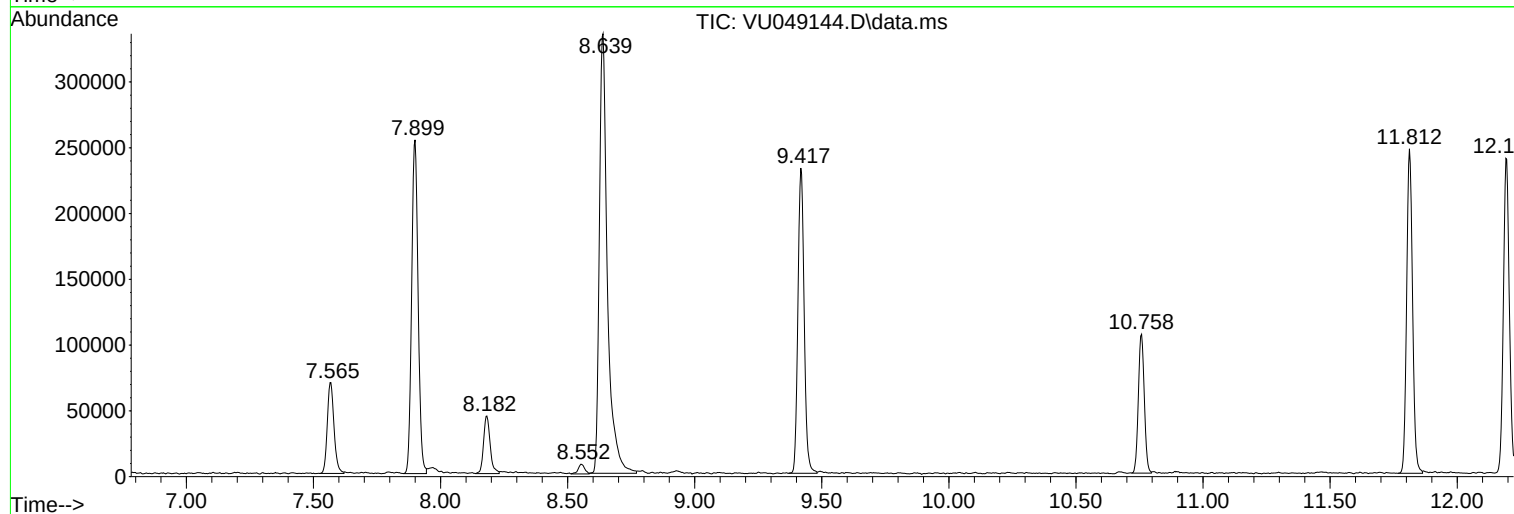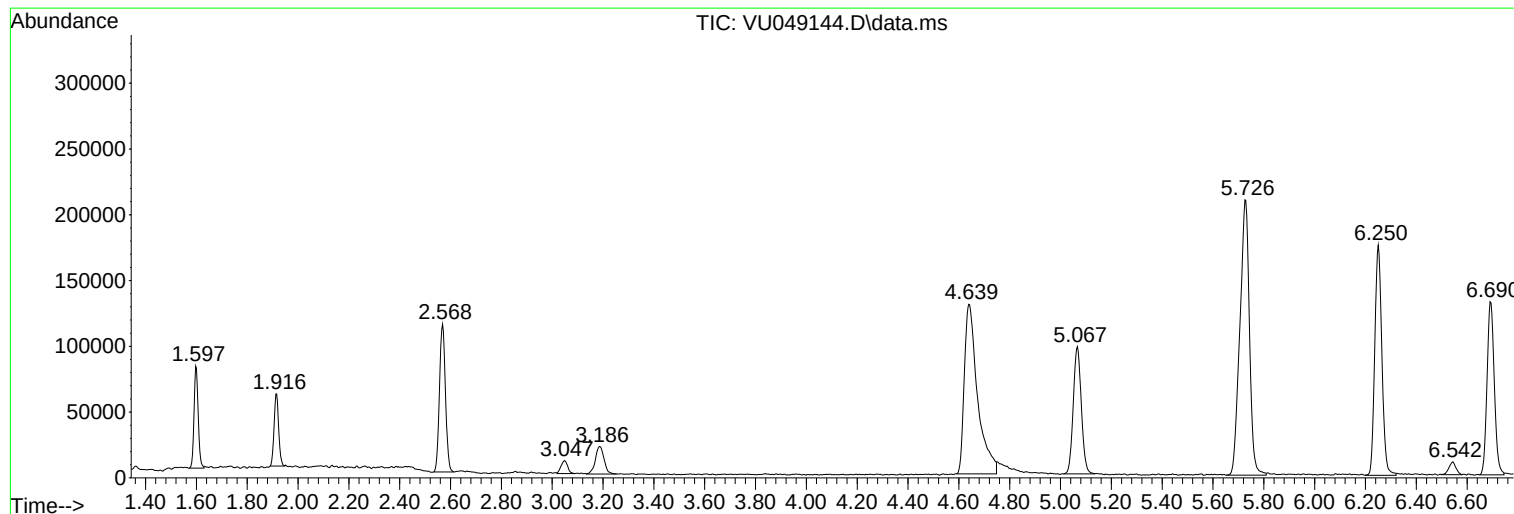

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049144.D
Acq On : 15 Jun 2022 03:39
Operator : SY/MD
Sample : N3274-10 250X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BA0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049144.D
Acq On : 15 Jun 2022 03:39
Operator : SY/MD
Sample : N3274-10 250X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BA0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc