

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
 Data File : VU049146.D
 Acq On : 15 Jun 2022 04:26
 Operator : SY/MD
 Sample : N3274-12 250X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BA2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU049146.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	96	rBV	75613	88309	12.22%	1.780%
2	1.916	169	179	193	rBV	55706	74134	10.25%	1.495%
3	2.568	370	382	399	rBV	111344	180567	24.98%	3.640%
4	3.051	519	532	543	rVB2	11621	22319	3.09%	0.450%
5	3.189	560	575	595	rVB	21302	48594	6.72%	0.980%
6	4.642	1010	1027	1063	rBV3	121272	451758	62.49%	9.108%
7	5.067	1144	1159	1177	rBV	95178	212946	29.46%	4.293%
8	5.726	1340	1364	1386	rBV3	201056	530499	73.38%	10.695%
9	6.250	1510	1527	1550	rBV	172722	335947	46.47%	6.773%
10	6.546	1606	1619	1632	rBV7	10077	20790	2.88%	0.419%
11	6.690	1648	1664	1684	rBV	126815	254567	35.21%	5.132%
12	7.568	1924	1937	1958	rBV	68006	125765	17.40%	2.536%
13	7.899	2026	2040	2056	rBV	249934	438877	60.71%	8.848%
14	7.967	2056	2061	2074	rVB2	4300	8615	1.19%	0.174%
15	8.182	2117	2128	2147	rBV	43140	77045	10.66%	1.553%
16	8.552	2232	2243	2255	rBV2	16492	28652	3.96%	0.578%
17	8.636	2257	2269	2304	rBV3	317125	722908	100.00%	14.574%
18	9.417	2495	2512	2527	rBV	233402	392916	54.35%	7.922%
19	10.758	2917	2929	2942	rVB	104067	165883	22.95%	3.344%
20	11.812	3244	3257	3276	rBV	241797	393670	54.46%	7.937%
21	12.195	3361	3376	3395	rBV	233729	385332	53.30%	7.769%




Sum of corrected areas: 4960093

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049146.D
Acq On : 15 Jun 2022 04:26
Operator : SY/MD
Sample : N3274-12 250X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BA2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

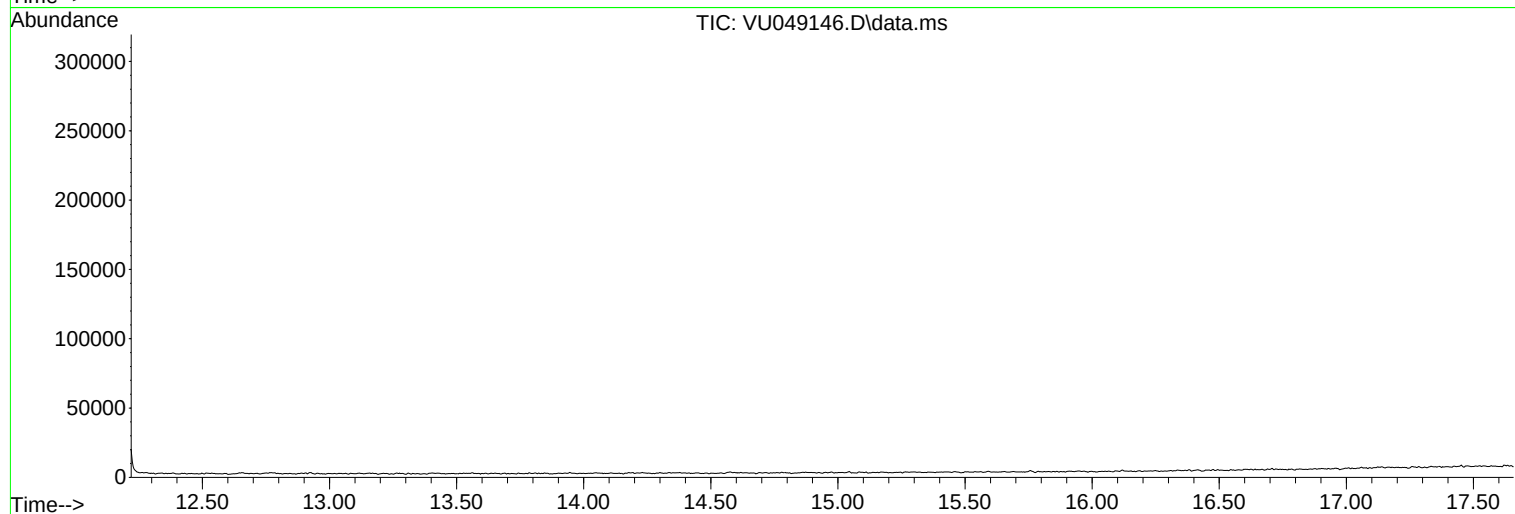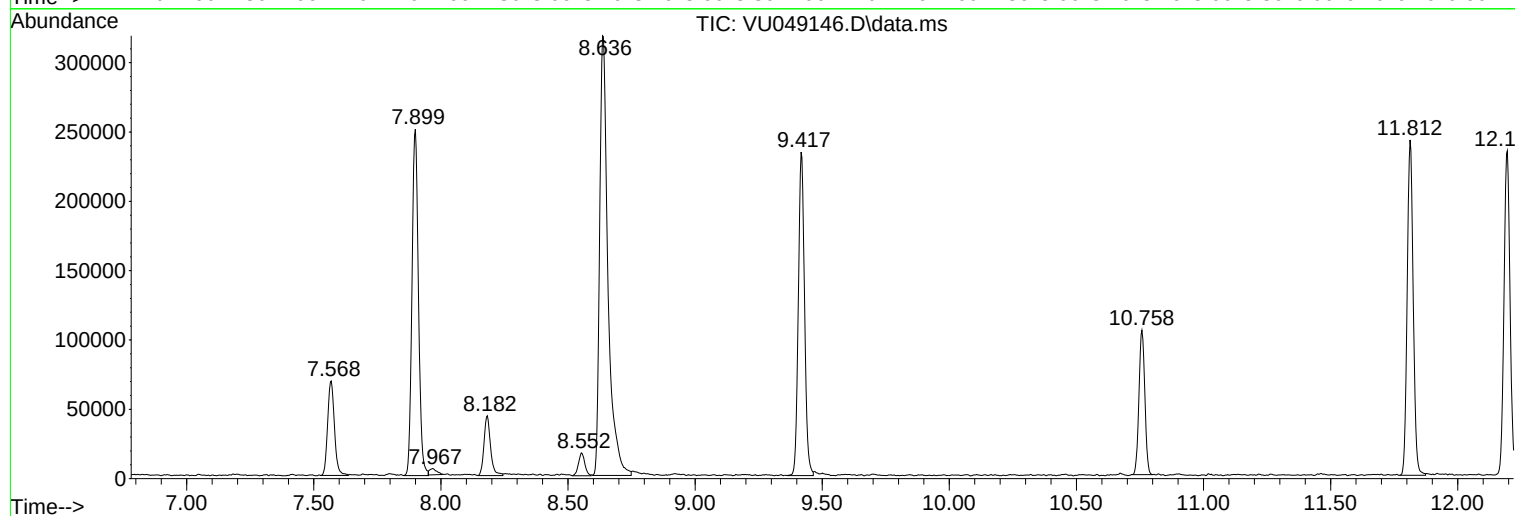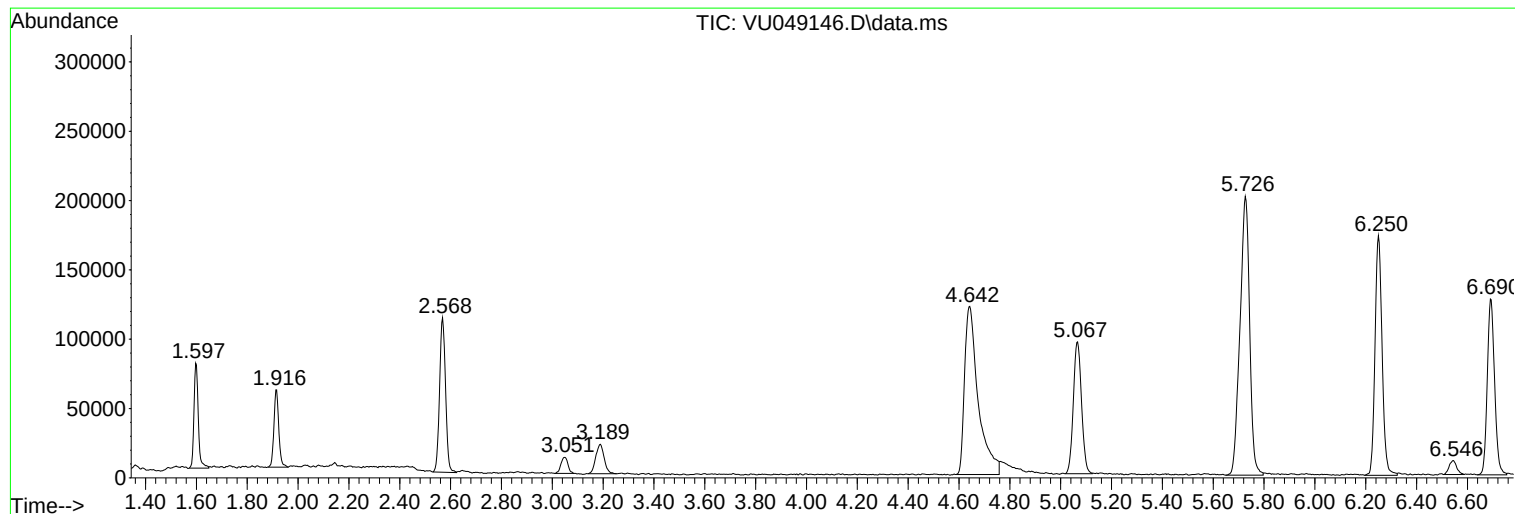

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049146.D
Acq On : 15 Jun 2022 04:26
Operator : SY/MD
Sample : N3274-12 250X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BA2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049146.D
Acq On : 15 Jun 2022 04:26
Operator : SY/MD
Sample : N3274-12 250X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BA2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc