

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
 Data File : VU049147.D
 Acq On : 15 Jun 2022 04:50
 Operator : SY/MD
 Sample : N3274-13 250X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BA3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU049147.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	98	rBV	77818	86966	11.55%	1.767%
2	1.916	171	179	193	rVB	55387	72795	9.67%	1.479%
3	2.568	371	382	398	rVB	110808	178609	23.73%	3.628%
4	3.047	520	531	542	rBV2	8856	16206	2.15%	0.329%
5	3.189	557	575	589	rBV	21746	49548	6.58%	1.007%
6	4.639	1008	1026	1068	rBV4	122736	468558	62.25%	9.519%
7	5.067	1143	1159	1177	rBV	96965	215607	28.65%	4.380%
8	5.726	1341	1364	1390	rBV2	206128	541222	71.91%	10.995%
9	6.250	1513	1527	1545	rBV	162195	310560	41.26%	6.309%
10	6.546	1604	1619	1629	rBV10	5673	12412	1.65%	0.252%
11	6.693	1651	1665	1685	rBV	128542	252312	33.52%	5.126%
12	7.568	1926	1937	1953	rBV	69559	123542	16.41%	2.510%
13	7.899	2027	2040	2057	rBV	255965	446158	59.28%	9.064%
14	8.182	2116	2128	2140	rBV	43253	75831	10.08%	1.541%
15	8.555	2235	2244	2255	rBV3	9671	16011	2.13%	0.325%
16	8.639	2257	2270	2305	rBV2	333424	752664	100.00%	15.290%
17	9.417	2500	2512	2532	rBV	216048	371974	49.42%	7.557%
18	10.758	2916	2929	2947	rVB	105819	173050	22.99%	3.516%
19	11.812	3245	3257	3277	rBV	229681	366673	48.72%	7.449%
20	12.195	3363	3376	3394	rBV	233536	391747	52.05%	7.958%




Sum of corrected areas: 4922445

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049147.D
Acq On : 15 Jun 2022 04:50
Operator : SY/MD
Sample : N3274-13 250X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BA3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

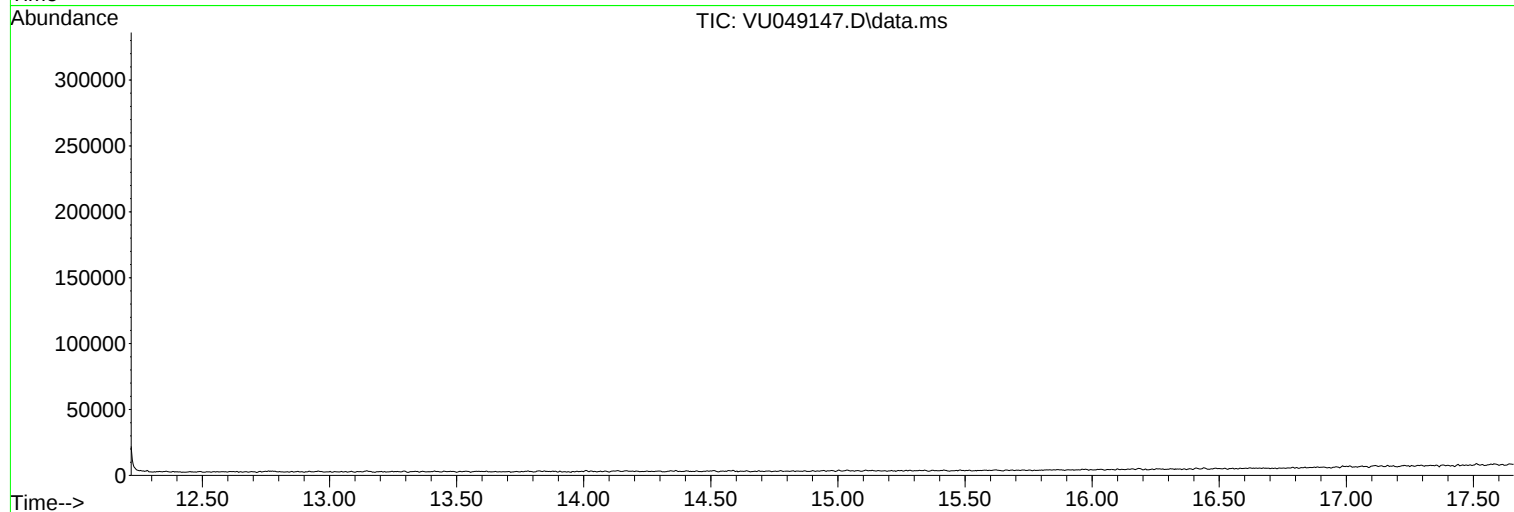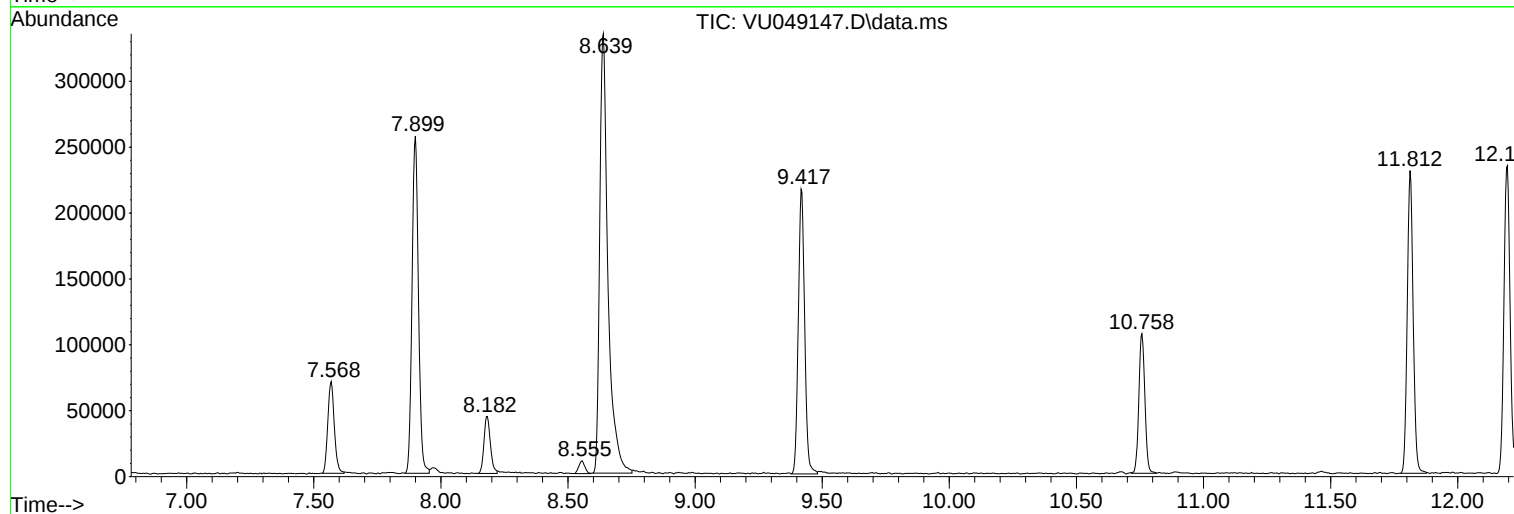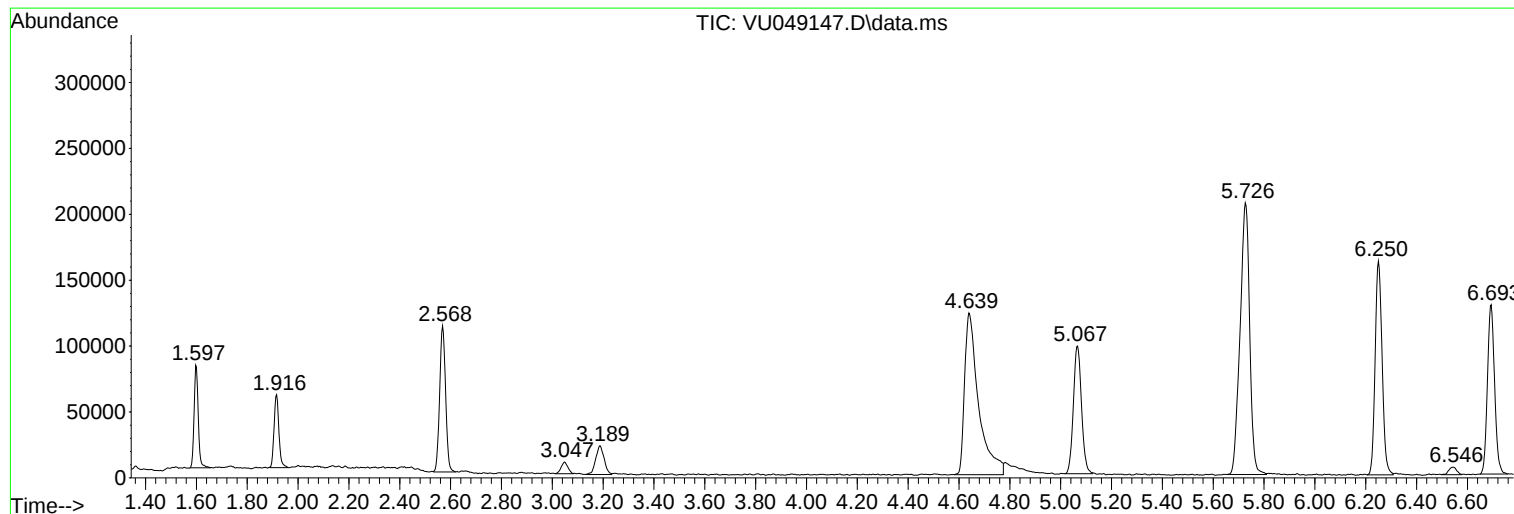

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049147.D
Acq On : 15 Jun 2022 04:50
Operator : SY/MD
Sample : N3274-13 250X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BA3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049147.D
Acq On : 15 Jun 2022 04:50
Operator : SY/MD
Sample : N3274-13 250X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BA3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc