

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
 Data File : VU049148.D
 Acq On : 15 Jun 2022 05:13
 Operator : SY/MD
 Sample : N3274-14 250X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BB7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU049148.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	98	rVB	73978	83575	11.42%	1.695%
2	1.913	170	178	190	rBV	55549	71442	9.76%	1.449%
3	2.568	367	382	397	rBV	109188	180478	24.67%	3.661%
4	3.048	523	531	542	rVB4	8113	14196	1.94%	0.288%
5	3.189	557	575	588	rBV	25391	59495	8.13%	1.207%
6	4.639	1010	1026	1066	rBV3	133885	491401	67.17%	9.969%
7	5.067	1142	1159	1178	rBV	95763	210324	28.75%	4.267%
8	5.726	1344	1364	1384	rBV2	200137	525936	71.89%	10.669%
9	6.250	1514	1527	1545	rBV2	163835	316314	43.23%	6.417%
10	6.543	1607	1618	1631	rVB5	13392	26930	3.68%	0.546%
11	6.690	1649	1664	1683	rBV	125544	252674	34.54%	5.126%
12	7.568	1923	1937	1956	rBV	68476	125918	17.21%	2.554%
13	7.899	2027	2040	2055	rBV	251617	437209	59.76%	8.869%
14	7.967	2057	2061	2074	rVB4	4200	7782	1.06%	0.158%
15	8.182	2118	2128	2142	rBV	40782	74177	10.14%	1.505%
16	8.555	2233	2244	2255	rVB	11467	19378	2.65%	0.393%
17	8.636	2255	2269	2310	rBV2	328337	731631	100.00%	14.842%
18	9.417	2500	2512	2532	rBV	223639	378514	51.74%	7.679%
19	10.758	2917	2929	2947	rVB	101825	168167	22.99%	3.411%
20	11.812	3245	3257	3275	rBV	229176	372188	50.87%	7.550%
21	12.195	3362	3376	3391	rBV	229770	381781	52.18%	7.745%




Sum of corrected areas: 4929510

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049148.D
Acq On : 15 Jun 2022 05:13
Operator : SY/MD
Sample : N3274-14 250X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BB7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

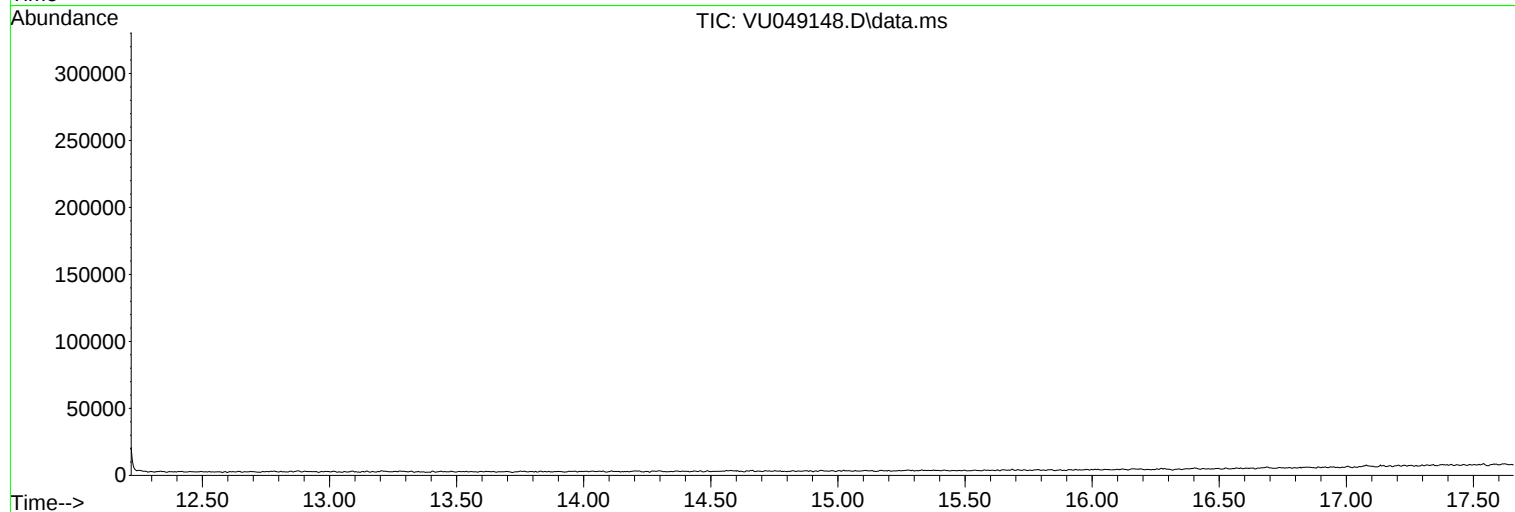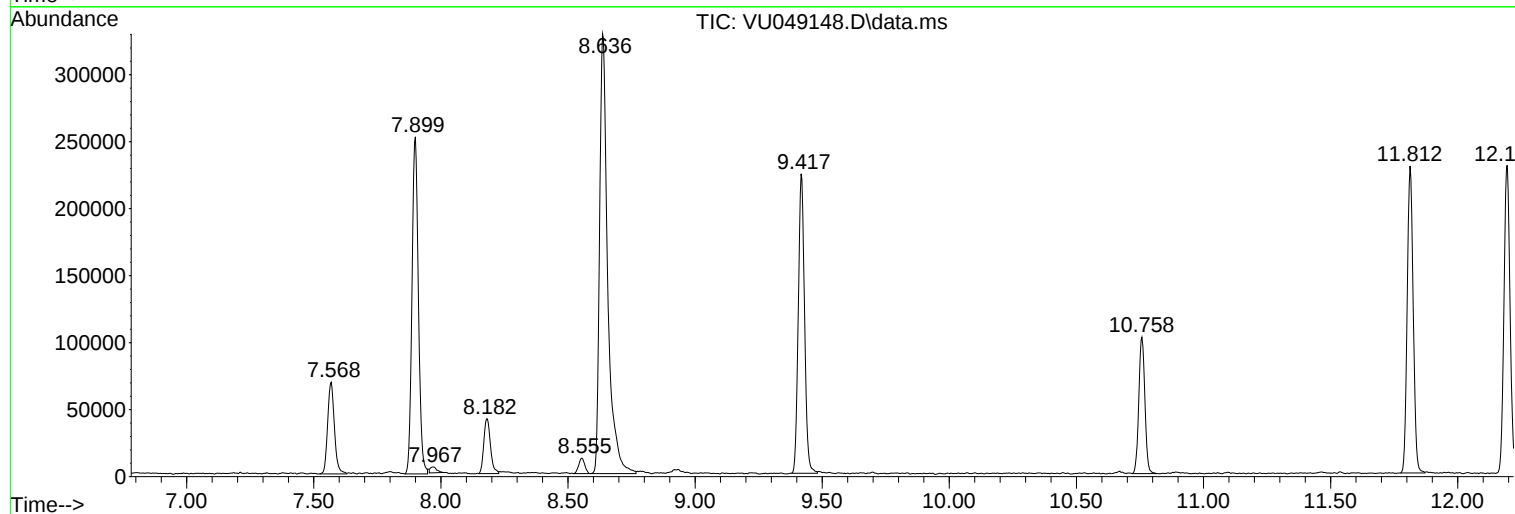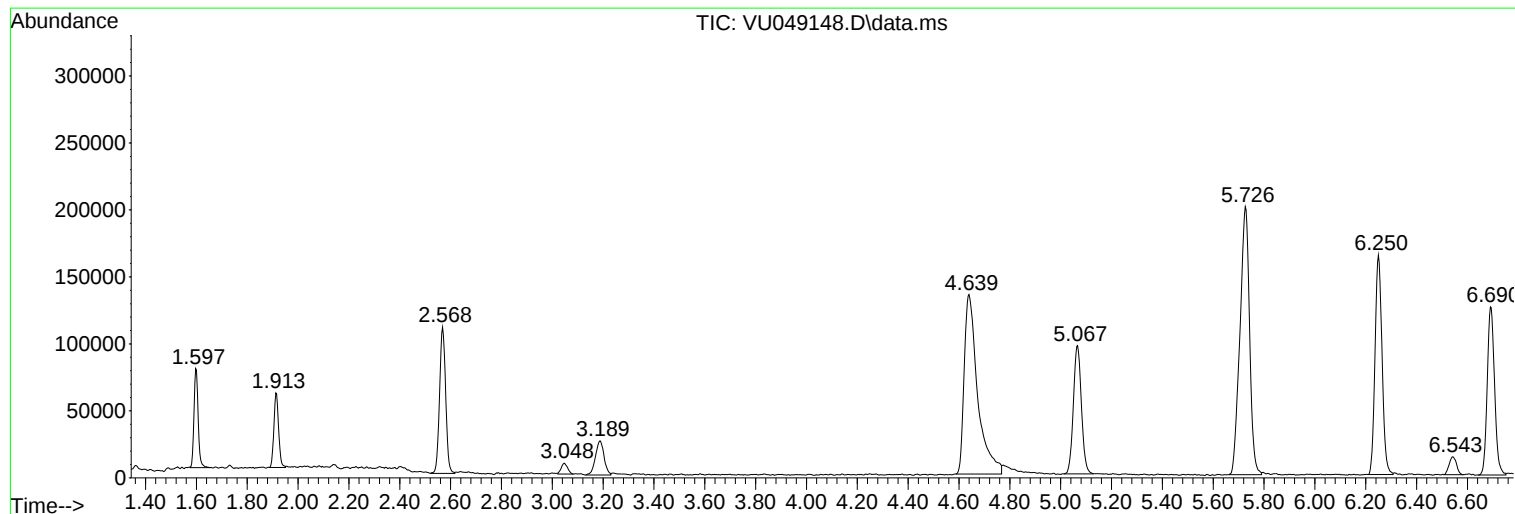

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049148.D
Acq On : 15 Jun 2022 05:13
Operator : SY/MD
Sample : N3274-14 250X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BB7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049148.D
Acq On : 15 Jun 2022 05:13
Operator : SY/MD
Sample : N3274-14 250X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BB7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
