

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
 Data File : VU049150.D
 Acq On : 15 Jun 2022 06:01
 Operator : SY/MD
 Sample : N3274-16 250X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BB9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU049150.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	94	rVB	75881	85348	11.22%	1.691%
2	1.916	170	179	190	rBV	56078	73367	9.65%	1.454%
3	2.568	370	382	397	rVB	113487	183644	24.15%	3.639%
4	3.044	518	530	543	rBV2	6382	12375	1.63%	0.245%
5	3.189	560	575	592	rBV	21599	50840	6.68%	1.007%
6	4.639	1010	1026	1064	rBV3	126998	476558	62.66%	9.442%
7	5.067	1143	1159	1182	rVB	99123	218821	28.77%	4.336%
8	5.726	1338	1364	1391	rBV2	208352	548473	72.11%	10.867%
9	6.250	1513	1527	1549	rBV	170558	326821	42.97%	6.475%
10	6.542	1606	1618	1630	rBV4	15504	30230	3.97%	0.599%
11	6.694	1646	1665	1684	rBV	133344	262635	34.53%	5.204%
12	7.568	1922	1937	1951	rBV	68875	126423	16.62%	2.505%
13	7.899	2026	2040	2055	rBV	256581	455175	59.85%	9.018%
14	8.182	2116	2128	2147	rBV	42025	77611	10.20%	1.538%
15	8.555	2236	2244	2252	rVB6	4795	7939	1.04%	0.157%
16	8.639	2257	2270	2310	rBV2	329859	760559	100.00%	15.069%
17	9.417	2500	2512	2532	rBV	228699	385129	50.64%	7.631%
18	10.758	2914	2929	2944	rBV	109057	179566	23.61%	3.558%
19	11.812	3245	3257	3273	rBV	239904	387472	50.95%	7.677%
20	12.192	3363	3375	3393	rBV	241732	398159	52.35%	7.889%




Sum of corrected areas: 5047145

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049150.D
Acq On : 15 Jun 2022 06:01
Operator : SY/MD
Sample : N3274-16 250X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BB9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

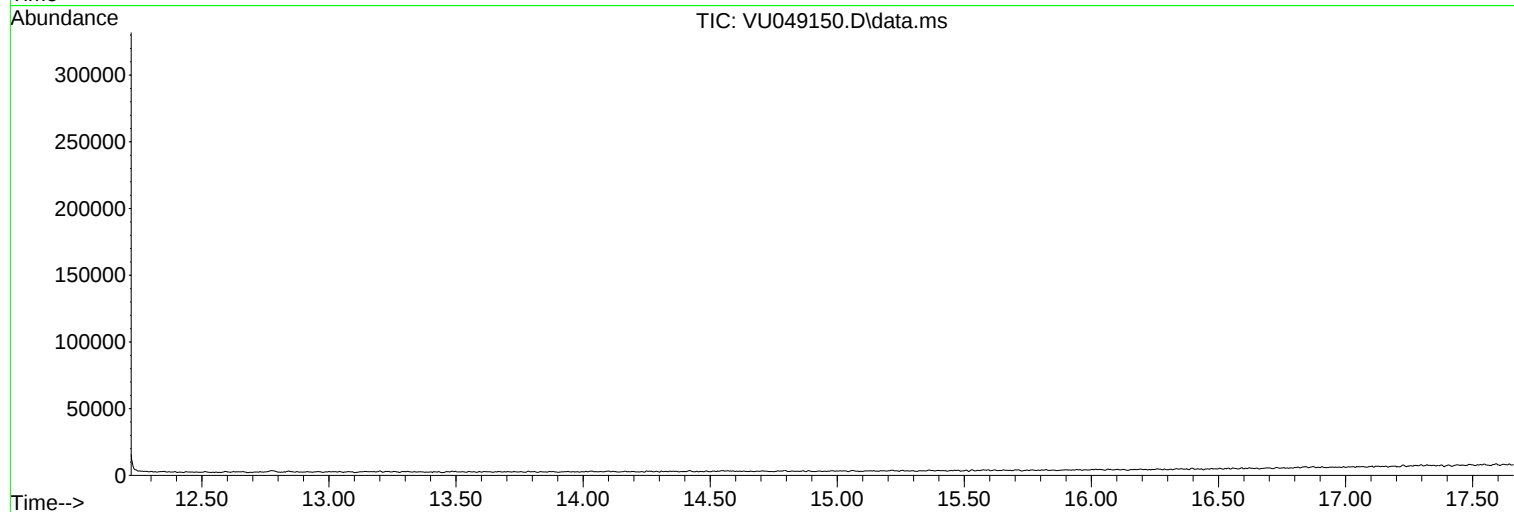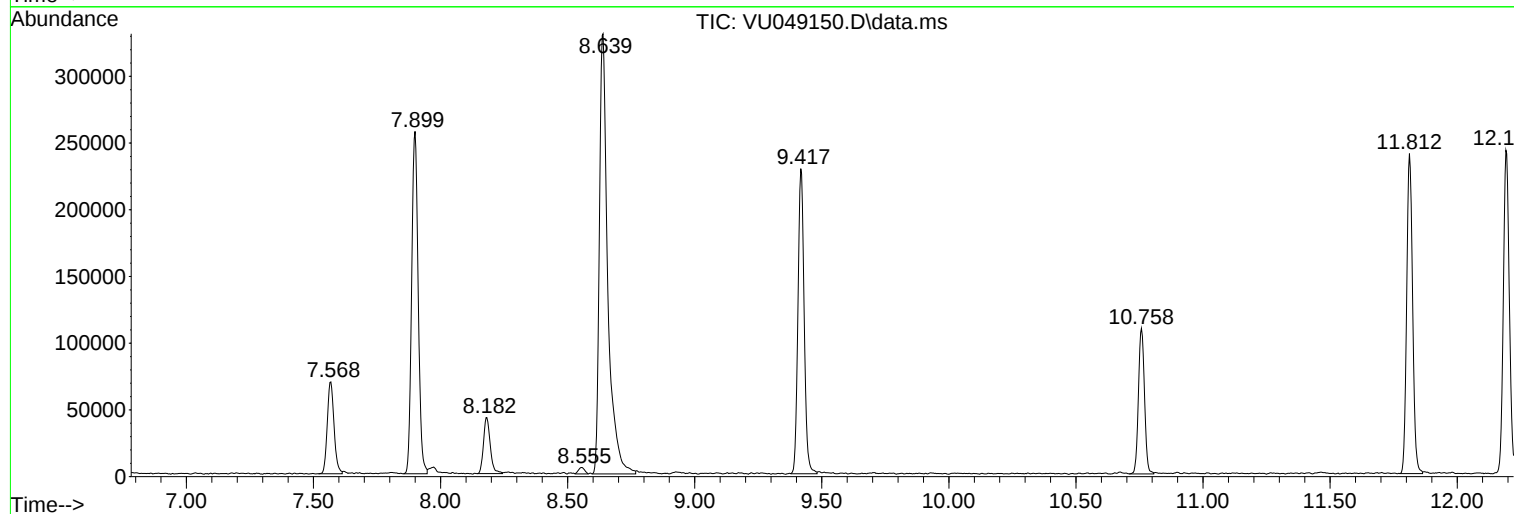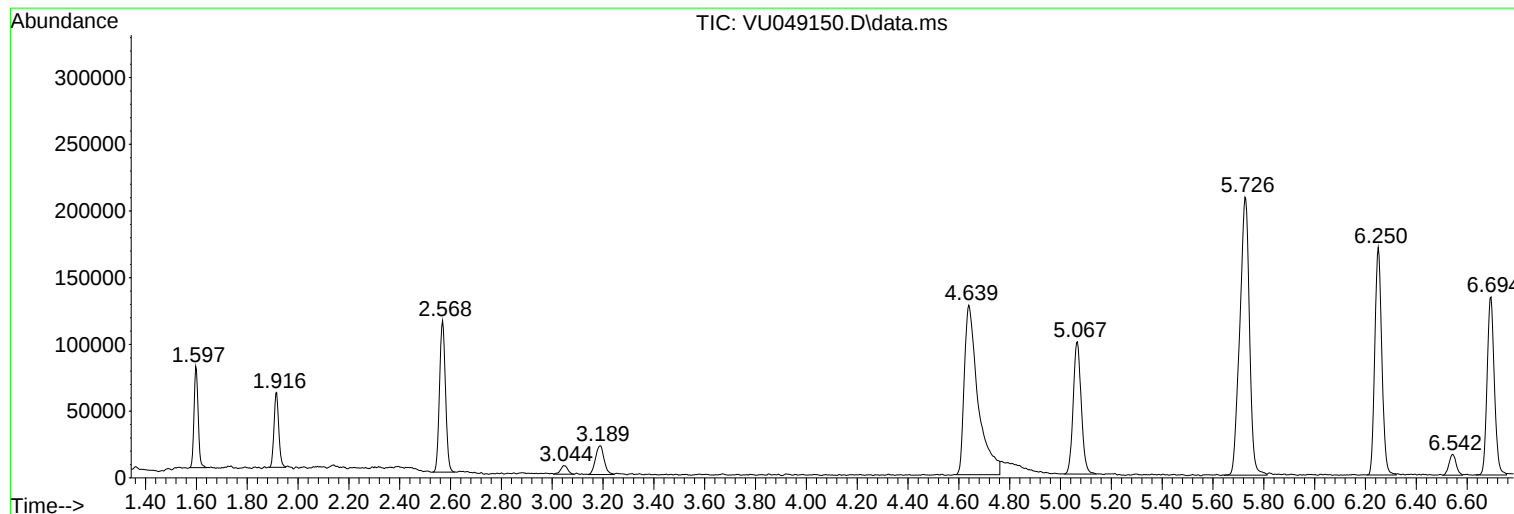

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049150.D
Acq On : 15 Jun 2022 06:01
Operator : SY/MD
Sample : N3274-16 250X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BB9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049150.D
Acq On : 15 Jun 2022 06:01
Operator : SY/MD
Sample : N3274-16 250X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BB9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc