

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
 Data File : VU049151.D
 Acq On : 15 Jun 2022 06:24
 Operator : SY/MD
 Sample : N3274-17 250X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BC0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU049151.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	94	rBV	74061	85405	11.70%	1.506%
2	1.916	170	179	191	rVB	56711	73048	10.01%	1.288%
3	2.138	243	248	257	rVB3	6824	9698	1.33%	0.171%
4	2.568	367	382	396	rBV	112163	180648	24.75%	3.186%
5	3.047	520	531	544	rBV2	8437	15229	2.09%	0.269%
6	3.186	561	574	589	rBV	20743	47299	6.48%	0.834%
7	4.639	1010	1026	1084	rBV2	128483	499359	68.43%	8.808%
8	5.067	1144	1159	1178	rBV	96891	213400	29.24%	3.764%
9	5.726	1344	1364	1387	rBV2	204937	534798	73.28%	9.433%
10	6.250	1515	1527	1546	rBV	168046	321260	44.02%	5.666%
11	6.542	1602	1618	1641	rBV	370619	708137	97.04%	12.490%
12	6.694	1652	1665	1688	rVB	128661	254764	34.91%	4.494%
13	7.568	1921	1937	1954	rBV	68208	124909	17.12%	2.203%
14	7.899	2027	2040	2056	rBV	255268	443088	60.72%	7.815%
15	8.182	2115	2128	2146	rBV	41565	75895	10.40%	1.339%
16	8.555	2233	2244	2256	rBV2	19362	33910	4.65%	0.598%
17	8.636	2256	2269	2309	rBV2	325481	729767	100.00%	12.872%
18	9.417	2499	2512	2532	rBV	226154	380332	52.12%	6.708%
19	10.758	2916	2929	2945	rBV	105395	169030	23.16%	2.981%
20	11.812	3242	3257	3272	rBV	236274	379784	52.04%	6.699%
21	12.192	3363	3375	3390	rBV2	234608	389723	53.40%	6.874%




Sum of corrected areas: 5669483

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049151.D
Acq On : 15 Jun 2022 06:24
Operator : SY/MD
Sample : N3274-17 250X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BC0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

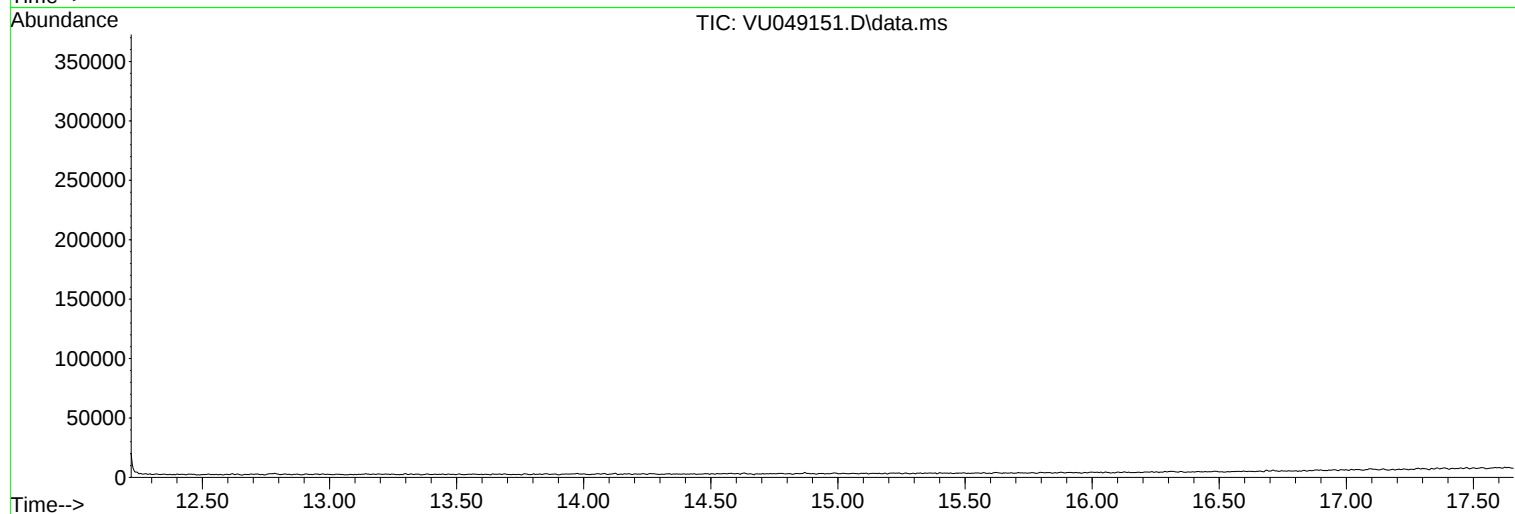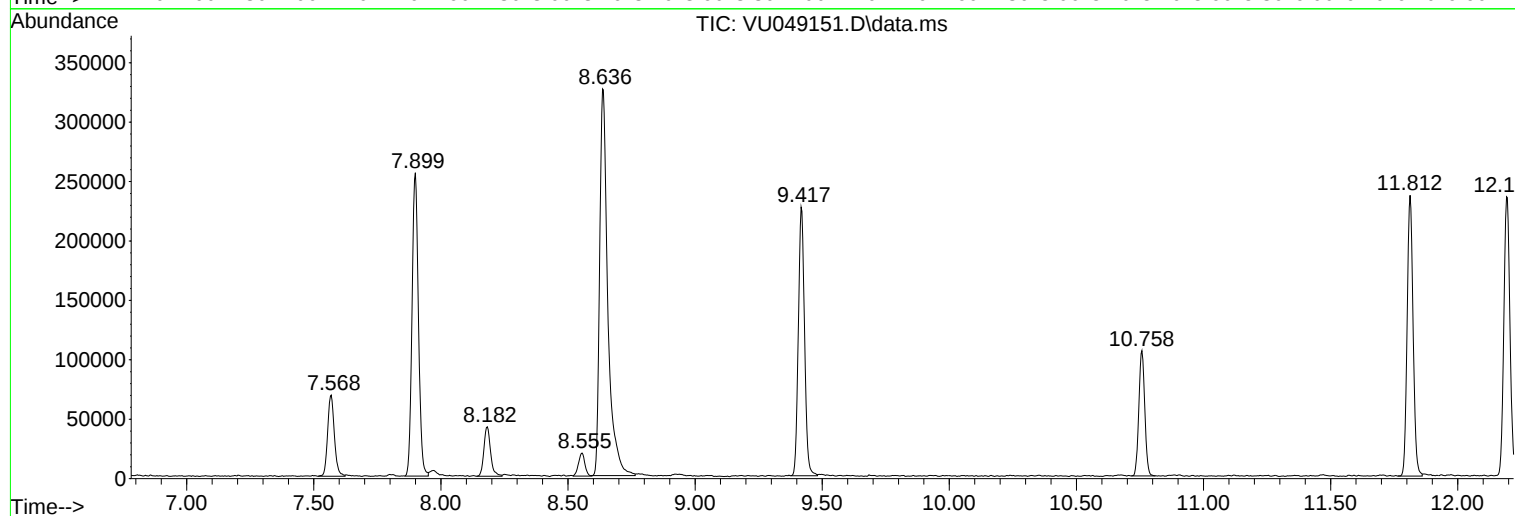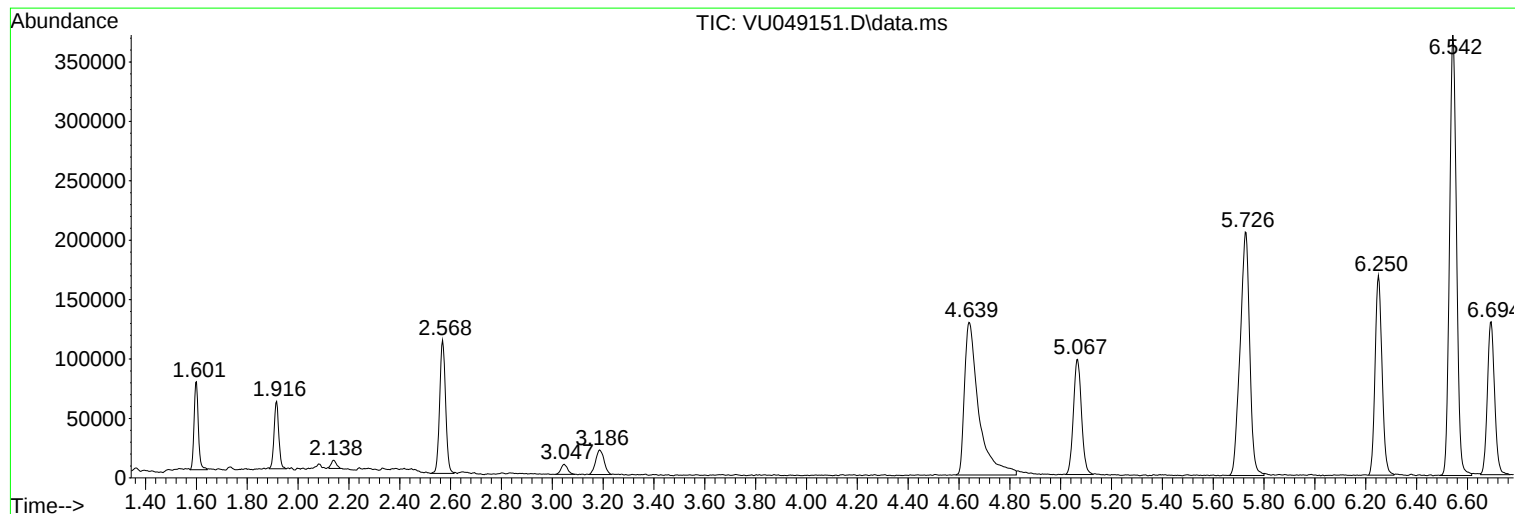

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049151.D
Acq On : 15 Jun 2022 06:24
Operator : SY/MD
Sample : N3274-17 250X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BC0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049151.D
Acq On : 15 Jun 2022 06:24
Operator : SY/MD
Sample : N3274-17 250X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BC0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
