

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
 Data File : VU049152.D
 Acq On : 15 Jun 2022 06:48
 Operator : SY/MD
 Sample : N3274-18 250X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BC1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU049152.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	93	rBV	73375	83353	11.42%	1.676%
2	1.916	171	179	188	rBV	53611	67571	9.26%	1.359%
3	2.568	371	382	401	rVB	107661	174917	23.97%	3.518%
4	3.047	521	531	543	rVB2	8356	16527	2.27%	0.332%
5	3.189	561	575	591	rVB	23562	53184	7.29%	1.070%
6	4.639	1009	1026	1061	rBV3	126167	466297	63.91%	9.378%
7	5.067	1143	1159	1177	rBV	92641	206615	28.32%	4.155%
8	5.726	1342	1364	1391	rBV2	198618	520232	71.30%	10.462%
9	6.250	1514	1527	1544	rBV	161779	312348	42.81%	6.282%
10	6.542	1605	1618	1633	rBV3	95688	181691	24.90%	3.654%
11	6.694	1650	1665	1682	rBV2	126440	249849	34.24%	5.025%
12	7.568	1921	1937	1953	rBV	65289	119781	16.42%	2.409%
13	7.899	2027	2040	2057	rBV	240841	424999	58.25%	8.547%
14	8.182	2116	2128	2142	rBV	40561	72506	9.94%	1.458%
15	8.636	2251	2269	2300	rBV2	321823	729598	100.00%	14.673%
16	9.417	2500	2512	2529	rBV	217564	370862	50.83%	7.458%
17	10.758	2916	2929	2946	rBV	103670	168455	23.09%	3.388%
18	11.812	3245	3257	3276	rBV	230045	372228	51.02%	7.486%
19	12.192	3364	3375	3397	rBV	230065	381459	52.28%	7.671%




Sum of corrected areas: 4972472

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049152.D
Acq On : 15 Jun 2022 06:48
Operator : SY/MD
Sample : N3274-18 250X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BC1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

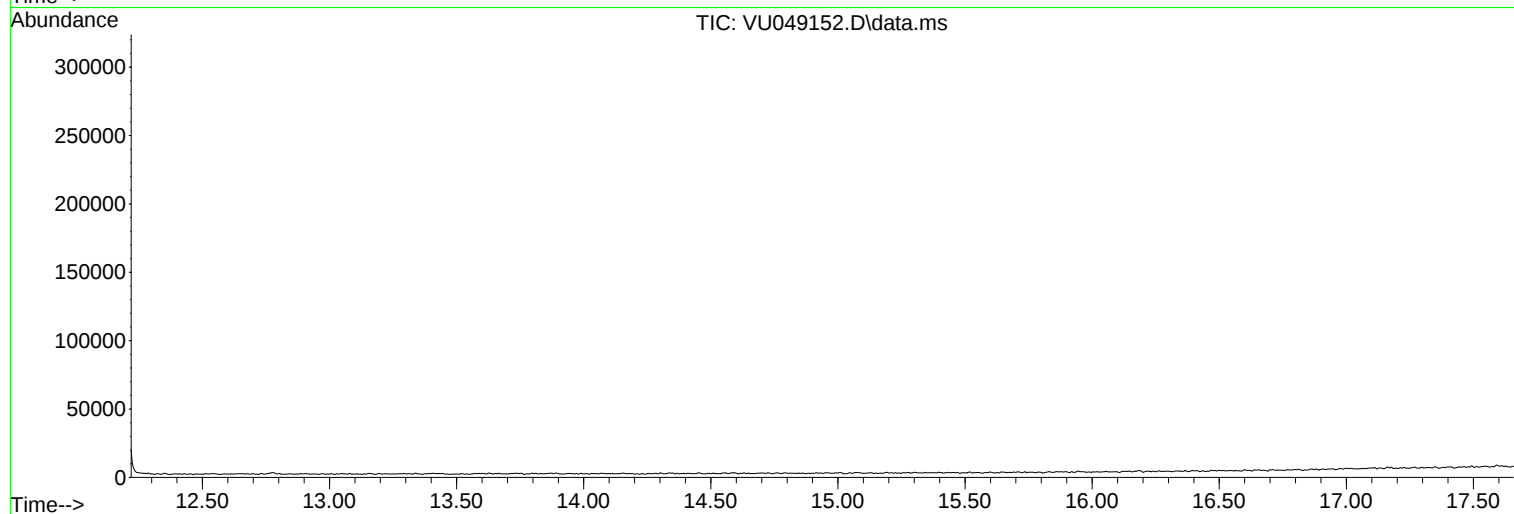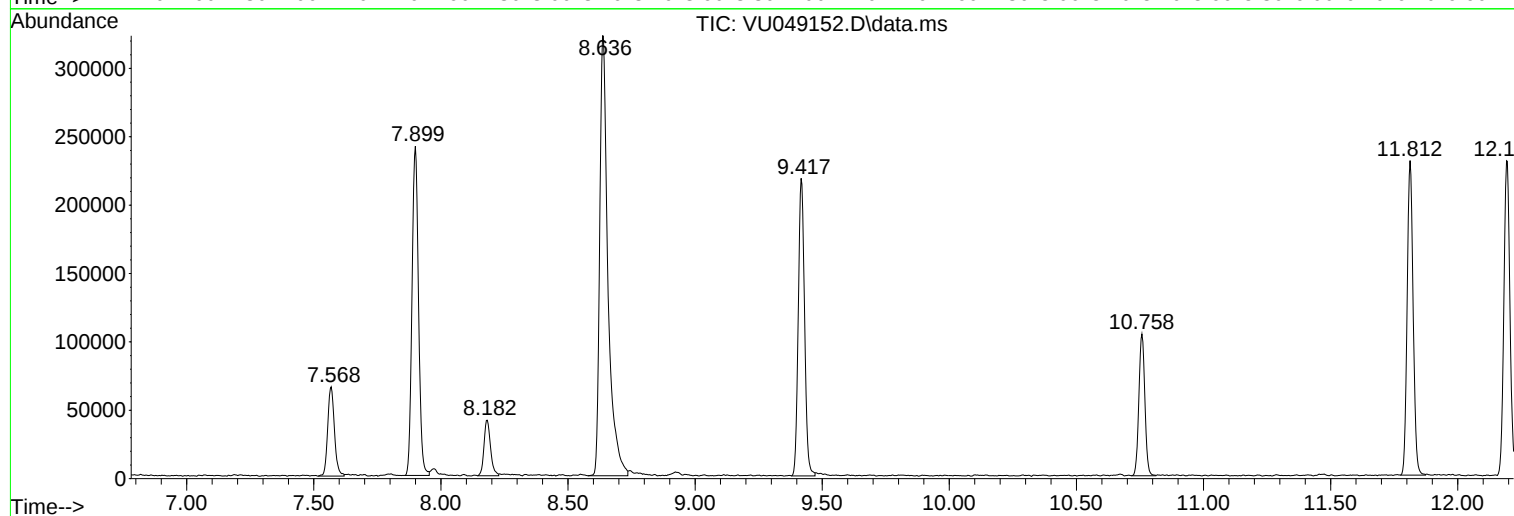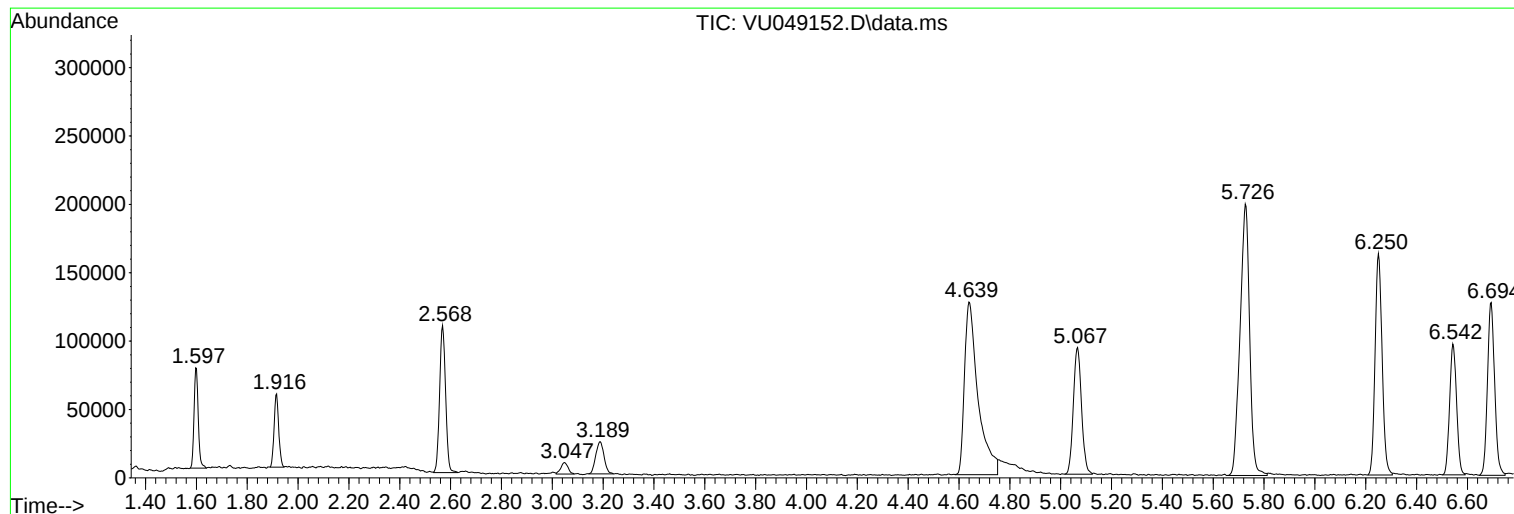

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049152.D
Acq On : 15 Jun 2022 06:48
Operator : SY/MD
Sample : N3274-18 250X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BC1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049152.D
Acq On : 15 Jun 2022 06:48
Operator : SY/MD
Sample : N3274-18 250X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BC1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc