

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
 Data File : VU049153.D
 Acq On : 15 Jun 2022 07:12
 Operator : SY/MD
 Sample : N3288-12 200X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGJA7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU049153.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	91	rBV	75886	86788	11.59%	1.772%
2	1.912	171	178	192	rVB	54725	70906	9.47%	1.448%
3	2.568	371	382	398	rVB	112313	182405	24.37%	3.724%
4	3.047	516	531	548	rBV2	20856	40836	5.46%	0.834%
5	3.186	561	574	587	rBV	17491	39154	5.23%	0.799%
6	4.639	1011	1026	1063	rBV2	110367	404264	54.00%	8.253%
7	5.066	1143	1159	1181	rVB2	97612	219637	29.34%	4.484%
8	5.726	1341	1364	1391	rBV2	205832	543726	72.63%	11.100%
9	6.250	1513	1527	1548	rBV	167151	320380	42.80%	6.540%
10	6.542	1602	1618	1632	rBV10	4728	11045	1.48%	0.225%
11	6.693	1650	1665	1686	rBV2	129285	258979	34.60%	5.287%
12	7.568	1923	1937	1951	rBV	67992	123633	16.52%	2.524%
13	7.899	2027	2040	2055	rBV	254768	446062	59.59%	9.106%
14	8.182	2117	2128	2148	rBV	41487	73649	9.84%	1.504%
15	8.635	2254	2269	2304	rBV2	342248	748576	100.00%	15.282%
16	9.417	2500	2512	2529	rBV	221554	381872	51.01%	7.796%
17	10.758	2918	2929	2945	rBV	106812	172016	22.98%	3.512%
18	11.812	3246	3257	3279	rBV	232695	380282	50.80%	7.763%
19	12.195	3362	3376	3391	rBV	238974	394223	52.66%	8.048%




Sum of corrected areas: 4898433

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049153.D
Acq On : 15 Jun 2022 07:12
Operator : SY/MD
Sample : N3288-12 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 54 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGJA7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

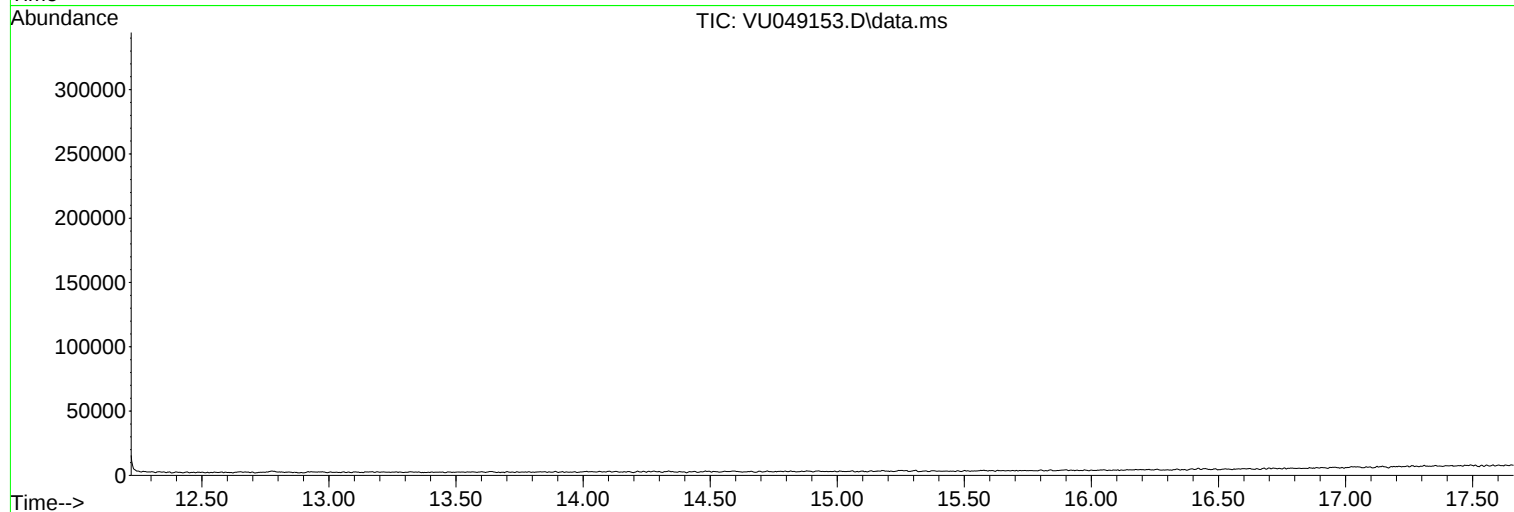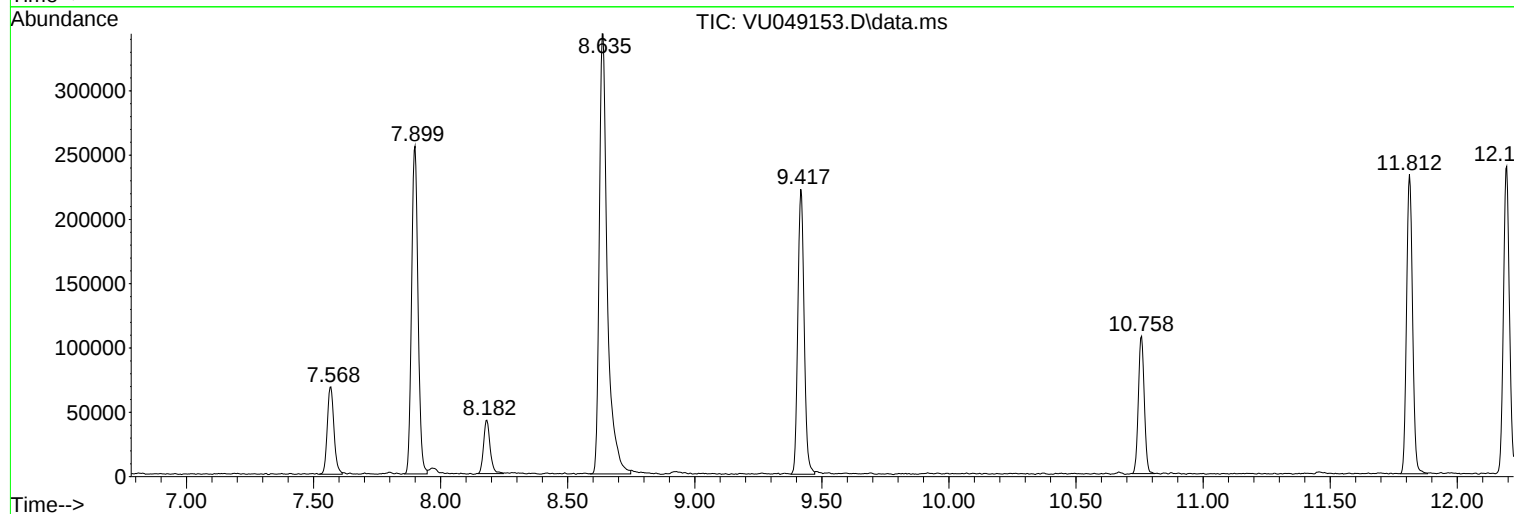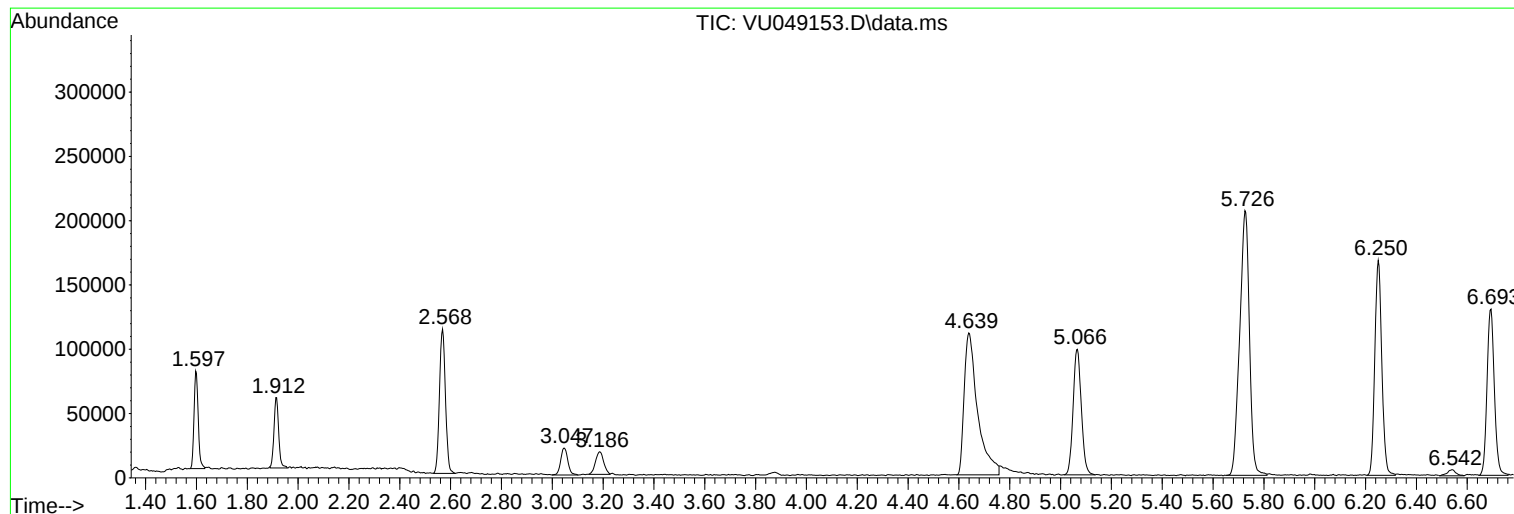

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049153.D
Acq On : 15 Jun 2022 07:12
Operator : SY/MD
Sample : N3288-12 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 54 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGJA7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049153.D
Acq On : 15 Jun 2022 07:12
Operator : SY/MD
Sample : N3288-12 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 54 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGJA7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc