


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061422\
Data File : VU049103.D
Acq On : 14 Jun 2022 09:42
Operator : SY/MD
Sample : BFB082
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB082

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Jun 17 02:27:54 2022

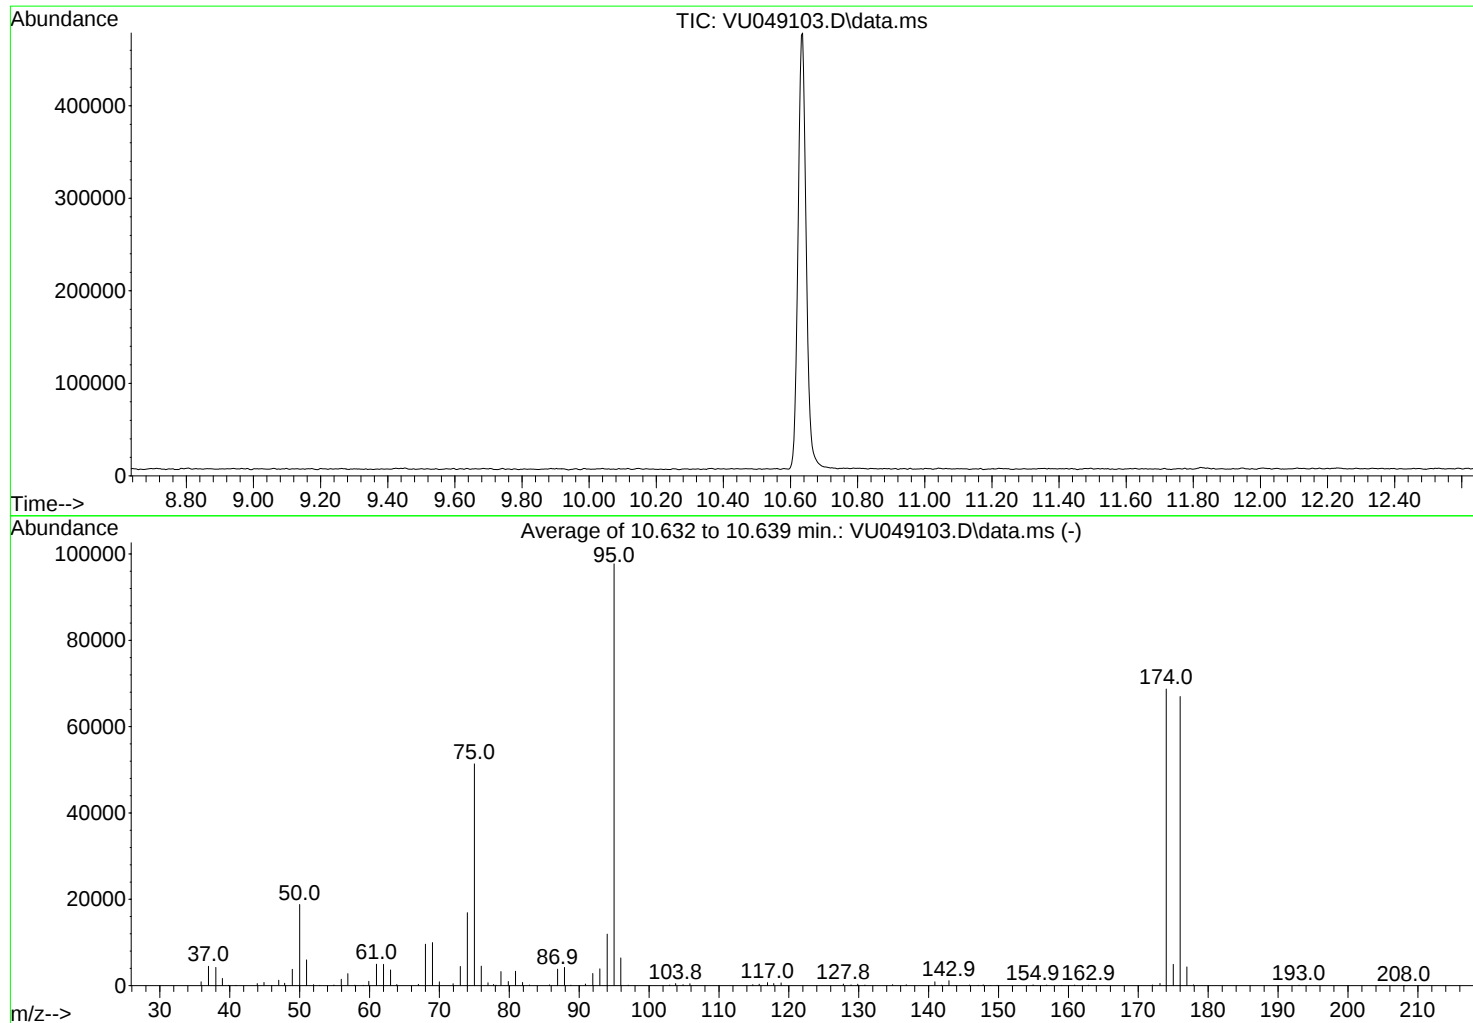

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	18803	PASS
75	95	30	80	52.6	51389	PASS
95	95	100	100	100.0	97720	PASS
96	95	5	9	6.6	6426	PASS
173	174	0.00	2	0.7	509	PASS
174	95	50	120	70.3	68709	PASS
175	174	5	9	7.2	4932	PASS
176	174	95	101	97.5	66987	PASS
177	176	5	9	6.5	4354	PASS

m/z	Abundance
38.90	152.0
39.80	239.0
40.90	207.0
41.90	153.0
43.00	339.0
43.90	1297.0
44.90	202.0
54.90	166.0
55.80	104.0
73.00	242.0
95.90	464.0
97.00	146.0
133.00	309.0
176.90	106.0
191.00	229.0
207.10	2322.0
208.00	497.0
209.00	308.0
281.10	204.0

Instrument :
MSVOA_U
ClientSampleId :
BFB082

m/z	Abundance
35.90	969.0
36.90	4675.0
38.00	4267.0
39.00	1787.0
39.90	285.0
40.90	283.0
41.90	124.0
42.90	378.0
44.00	1782.0
44.90	934.0
46.00	118.0
47.00	1302.0
47.90	609.0
49.00	3998.0
50.00	19160.0
51.00	6453.0
52.00	207.0
54.90	310.0
56.00	1694.0
56.90	2880.0
57.90	138.0
59.90	1007.0
61.00	5374.0
62.00	5052.0
63.00	3855.0
63.90	262.0
67.00	350.0
68.00	10048.0
69.00	10453.0
70.00	941.0
71.90	510.0
73.00	4902.0
74.00	17848.0
75.00	53360.0
76.00	4819.0
76.90	738.0
77.70	403.0
78.80	3228.0
79.90	1005.0
80.90	3485.0
81.90	734.0
82.90	155.0
85.80	174.0
86.90	4025.0
87.90	4210.0
88.80	105.0
90.90	456.0
92.00	2978.0
93.00	4133.0
94.00	12470.0
95.00	100304.0
96.00	7149.0
97.00	240.0
103.00	155.0
103.80	516.0
104.90	261.0
105.80	479.0
114.80	206.0
115.80	346.0
116.90	763.0
117.90	465.0
118.90	614.0
127.80	382.0
128.90	202.0
129.80	332.0
130.80	157.0
132.90	278.0
134.80	227.0
136.80	220.0
140.90	998.0
141.80	129.0
142.90	1170.0
143.90	106.0
145.90	141.0
147.80	188.0
148.90	131.0
149.80	148.0
155.00	164.0
156.80	104.0
159.00	117.0
160.80	122.0
162.90	125.0
172.10	183.0
174.00	68704.0
175.00	5104.0
176.00	67360.0
177.00	4602.0
177.90	150.0
191.00	175.0
193.00	120.0
207.10	2426.0
208.00	546.0

Instrument :
MSVOA_U
ClientSampleId :
BFB082

209.10243.0

281.10168.0

Instrument :
MSVOA_U
ClientSampleId :
BFB082

m/z	Abundance
35.90	922.0
37.00	4573.0
38.00	4390.0
39.00	1876.0
39.90	319.0
40.90	279.0
41.90	111.0
42.90	324.0
44.00	1801.0
44.90	937.0
47.00	1283.0
47.90	590.0
49.00	3863.0
50.00	19448.0
51.00	6150.0
52.00	196.0
52.90	105.0
55.00	333.0
56.00	1649.0
56.90	2846.0
57.90	136.0
59.10	113.0
59.90	1044.0
61.00	5118.0
62.00	5143.0
63.00	3728.0
63.90	248.0
67.00	288.0
68.00	9865.0
69.00	10276.0
70.00	931.0
71.90	433.0
73.00	4801.0
74.00	17368.0
75.00	53064.0
76.00	4728.0
76.90	717.0
77.80	352.0
78.80	3407.0
79.80	992.0
80.90	3431.0
81.90	766.0
82.90	143.0
85.70	190.0
86.90	3855.0
87.90	4389.0
88.80	120.0
90.90	375.0
92.00	2926.0
92.90	4032.0
94.00	12391.0
95.00	100664.0
96.00	7062.0
97.00	265.0
103.00	165.0
103.80	505.0
104.90	241.0
105.90	494.0
114.80	227.0
115.70	341.0
116.90	709.0
117.80	485.0
118.90	636.0
127.80	387.0
128.90	201.0
129.80	355.0
130.90	167.0
133.00	268.0
134.90	224.0
136.80	235.0
140.90	895.0
141.80	136.0
142.90	1201.0
145.90	154.0
147.10	105.0
147.80	213.0
149.80	124.0
155.00	171.0
156.90	133.0
160.90	139.0
162.90	128.0
172.10	144.0
173.10	776.0
174.00	70848.0
175.00	5096.0
176.00	69128.0
177.00	4587.0
177.90	189.0
191.00	168.0
193.00	122.0
207.10	2250.0
208.00	513.0

Instrument :
MSVOA_U
ClientSampleId :
BFB082

208.90254.0

281.10143.0

Instrument :
MSVOA_U
ClientSampleId :
BFB082

m/z	Abundance
35.90	785.0
37.00	4219.0
38.00	4076.0
39.00	1773.0
39.90	312.0
40.90	289.0
41.90	143.0
42.90	301.0
44.00	1780.0
45.00	941.0
47.00	1164.0
47.80	472.0
48.90	3516.0
50.00	17800.0
51.00	5356.0
52.00	233.0
52.90	113.0
55.00	347.0
56.00	1408.0
56.90	2660.0
57.90	116.0
59.10	111.0
59.90	1010.0
61.00	4392.0
62.00	4599.0
63.00	3291.0
63.90	245.0
67.00	224.0
68.00	8923.0
69.00	9198.0
70.00	795.0
72.00	366.0
73.00	4385.0
74.00	15526.0
75.00	47744.0
76.00	4057.0
77.00	601.0
78.10	367.0
78.80	3190.0
79.90	903.0
80.90	3143.0
81.90	735.0
82.90	139.0
85.70	154.0
86.90	3570.0
87.90	4115.0
88.80	124.0
90.90	309.0
91.90	2611.0
92.90	3497.0
94.00	10986.0
95.00	92192.0
96.00	6458.0
97.00	310.0
102.90	148.0
103.80	437.0
104.80	196.0
105.90	429.0
114.90	203.0
115.70	313.0
117.00	616.0
117.80	461.0
118.90	599.0
127.80	369.0
128.90	173.0
129.90	351.0
131.00	163.0
133.00	254.0
134.90	216.0
136.80	206.0
140.90	802.0
141.90	118.0
142.90	1039.0
145.80	163.0
147.10	118.0
147.80	202.0
154.90	174.0
157.00	165.0
161.00	136.0
162.90	110.0
172.00	124.0
173.10	750.0
174.00	66576.0
175.00	4595.0
176.00	64472.0
177.00	4190.0
177.90	174.0
191.10	212.0
193.00	102.0
207.00	2241.0
208.00	478.0
208.90	300.0

Instrument :
MSVOA_U
ClientSampleId :
BFB082

281.10

165.0

Instrument :
MSVOA_U
ClientSampleId :
BFB082