

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061424\
 Data File : VU059244.D
 Acq On : 14 Jun 2024 13:53
 Operator : MD/SY
 Sample : P2775-08ME
 Misc : 3.22g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Jun 15 02:51:20 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 15 02:48:14 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.238	114	219746	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	224778	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.810	152	102419	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.592	65	22256	16.916	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	33.840%#	
7) Chloroethane-d5	1.872	69	19852	17.614	ug/L	-0.04
Spiked Amount	50.000	Range 70 - 130	Recovery	=	35.220%#	
11) 1,1-Dichloroethene-d2	2.541	63	33343	12.839	ug/L	-0.02
Spiked Amount	50.000	Range 60 - 125	Recovery	=	25.680%#	
21) 2-Butanone-d5	4.621	46	99012	79.839	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	79.840%	
24) Chloroform-d	5.052	84	78051	29.799	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	59.600%#	
26) 1,2-Dichloroethane-d4	5.692	65	50418	31.406	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	62.820%#	
32) Benzene-d6	5.714	84	128292	24.868	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	49.740%#	
36) 1,2-Dichloropropane-d6	6.679	67	51404	28.898	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	57.800%#	
41) Toluene-d8	7.891	98	100007	22.835	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	45.680%#	
43) trans-1,3-Dichloroprop...	8.177	79	19447	27.046	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	54.100%#	
47) 2-Hexanone-d5	8.637	63	64954	78.964	ug/L	0.01
Spiked Amount	100.000	Range 45 - 130	Recovery	=	78.960%	
56) 1,1,2,2-Tetrachloroeth...	10.753	84	116001	38.532	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	77.060%	
66) 1,2-Dichlorobenzene-d4	12.190	152	53579	35.055	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	70.100%#	
Target Compounds						
					Qvalue	
15) Methyl Acetate	2.949	43	6508	2.819	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061424\
Data File : VU059244.D
Acq On : 14 Jun 2024 13:53
Operator : MD/SY
Sample : P2775-08ME
Misc : 3.22g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: Jun 15 02:51:20 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jun 15 02:48:14 2024
Response via : Initial Calibration

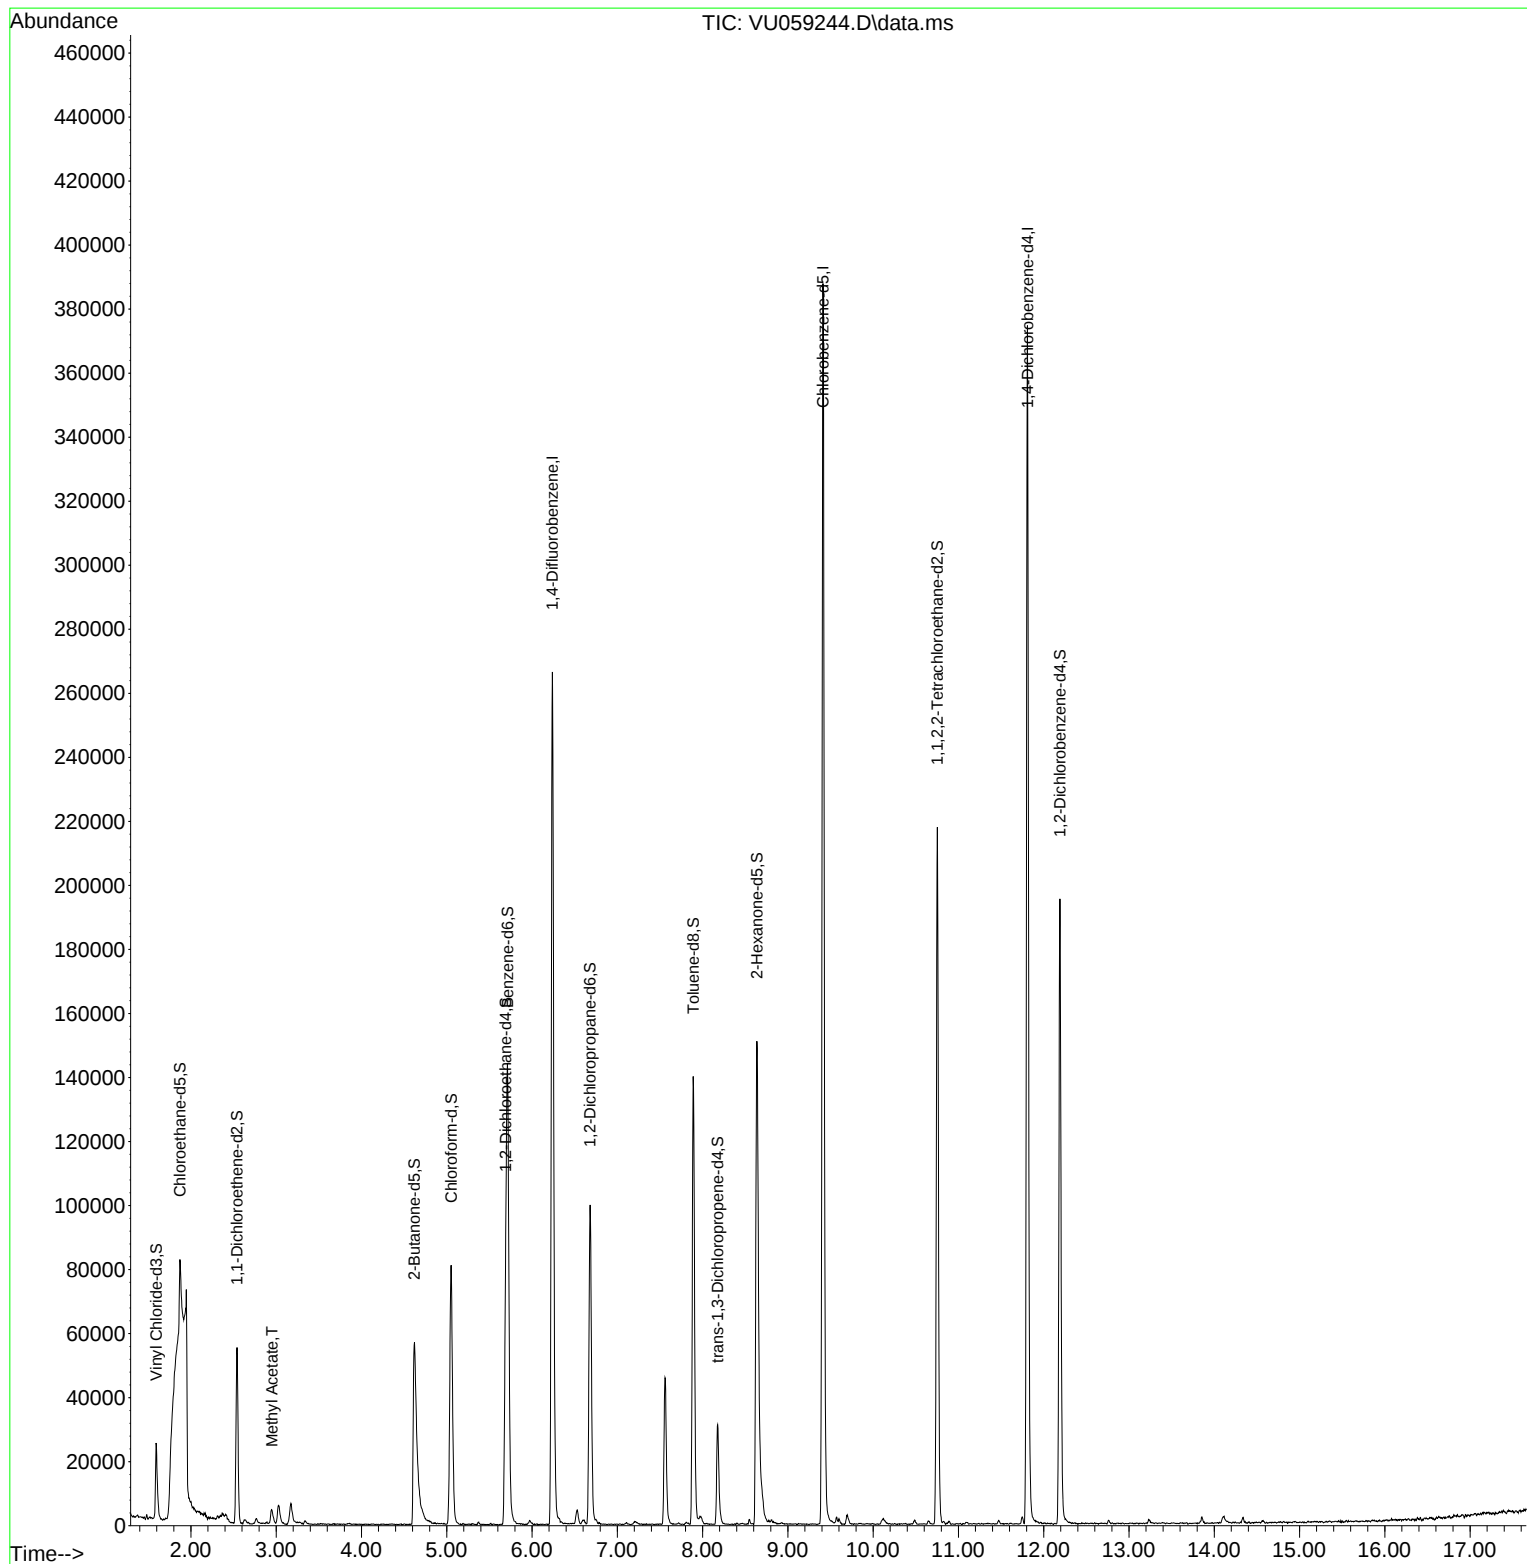

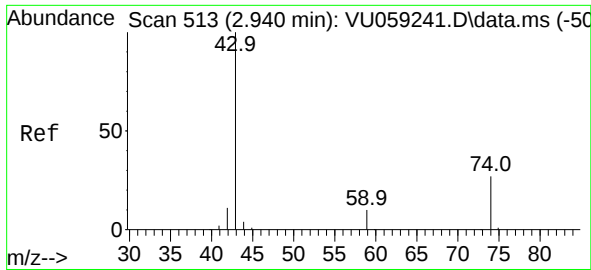

#15
Methyl Acetate
Concen: 2.819 ug/L
RT: 2.949 min Scan# 51
Delta R.T. 0.009 min
Lab File: VU059244.D
Acq: 14 Jun 2024 13:53

Instrument :
MSVOA_U
ClientSampleId :

Tgt Ion: 43 Resp: 6508
Ion Ratio Lower Upper
43 100
74 22.7 20.8 31.2

