

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061424\
 Data File : VU059245.D
 Acq On : 14 Jun 2024 14:15
 Operator : MD/SY
 Sample : P2775-09ME
 Misc : 3.51g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Jun 15 02:51:32 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 15 02:48:14 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.239	114	216563	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	221669	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.811	152	100372	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.593	65	22001	16.967	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	33.940%#		
7) Chloroethane-d5	1.872	69	19047	17.148	ug/L	-0.04
Spiked Amount 50.000	Range 70 - 130		Recovery =	34.300%#		
11) 1,1-Dichloroethene-d2	2.538	63	35135	13.728	ug/L	-0.03
Spiked Amount 50.000	Range 60 - 125		Recovery =	27.460%#		
21) 2-Butanone-d5	4.618	46	111205	90.989	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	90.990%		
24) Chloroform-d	5.052	84	78305	30.336	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	60.680%#		
26) 1,2-Dichloroethane-d4	5.692	65	51341	32.451	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	64.900%#		
32) Benzene-d6	5.715	84	133658	26.271	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	52.540%#		
36) 1,2-Dichloropropane-d6	6.683	67	54271	30.938	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	61.880%#		
41) Toluene-d8	7.891	98	100092	23.175	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	46.360%#		
43) trans-1,3-Dichloroprop...	8.178	79	19685	27.761	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	55.520%#		
47) 2-Hexanone-d5	8.641	63	67119	82.741	ug/L	0.02
Spiked Amount 100.000	Range 45 - 130		Recovery =	82.740%		
56) 1,1,2,2-Tetrachloroeth...	10.753	84	121475	40.916	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	81.840%		
66) 1,2-Dichlorobenzene-d4	12.190	152	54930	36.672	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	73.340%#		
Target Compounds						Qvalue
15) Methyl Acetate	2.943	43	8517	3.743	ug/L	97
37) 1,2-Dichloropropane	6.683	63	5808	2.555	ug/L #	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061424\
Data File : VU059245.D
Acq On : 14 Jun 2024 14:15
Operator : MD/SY
Sample : P2775-09ME
Misc : 3.51g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: Jun 15 02:51:32 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jun 15 02:48:14 2024
Response via : Initial Calibration




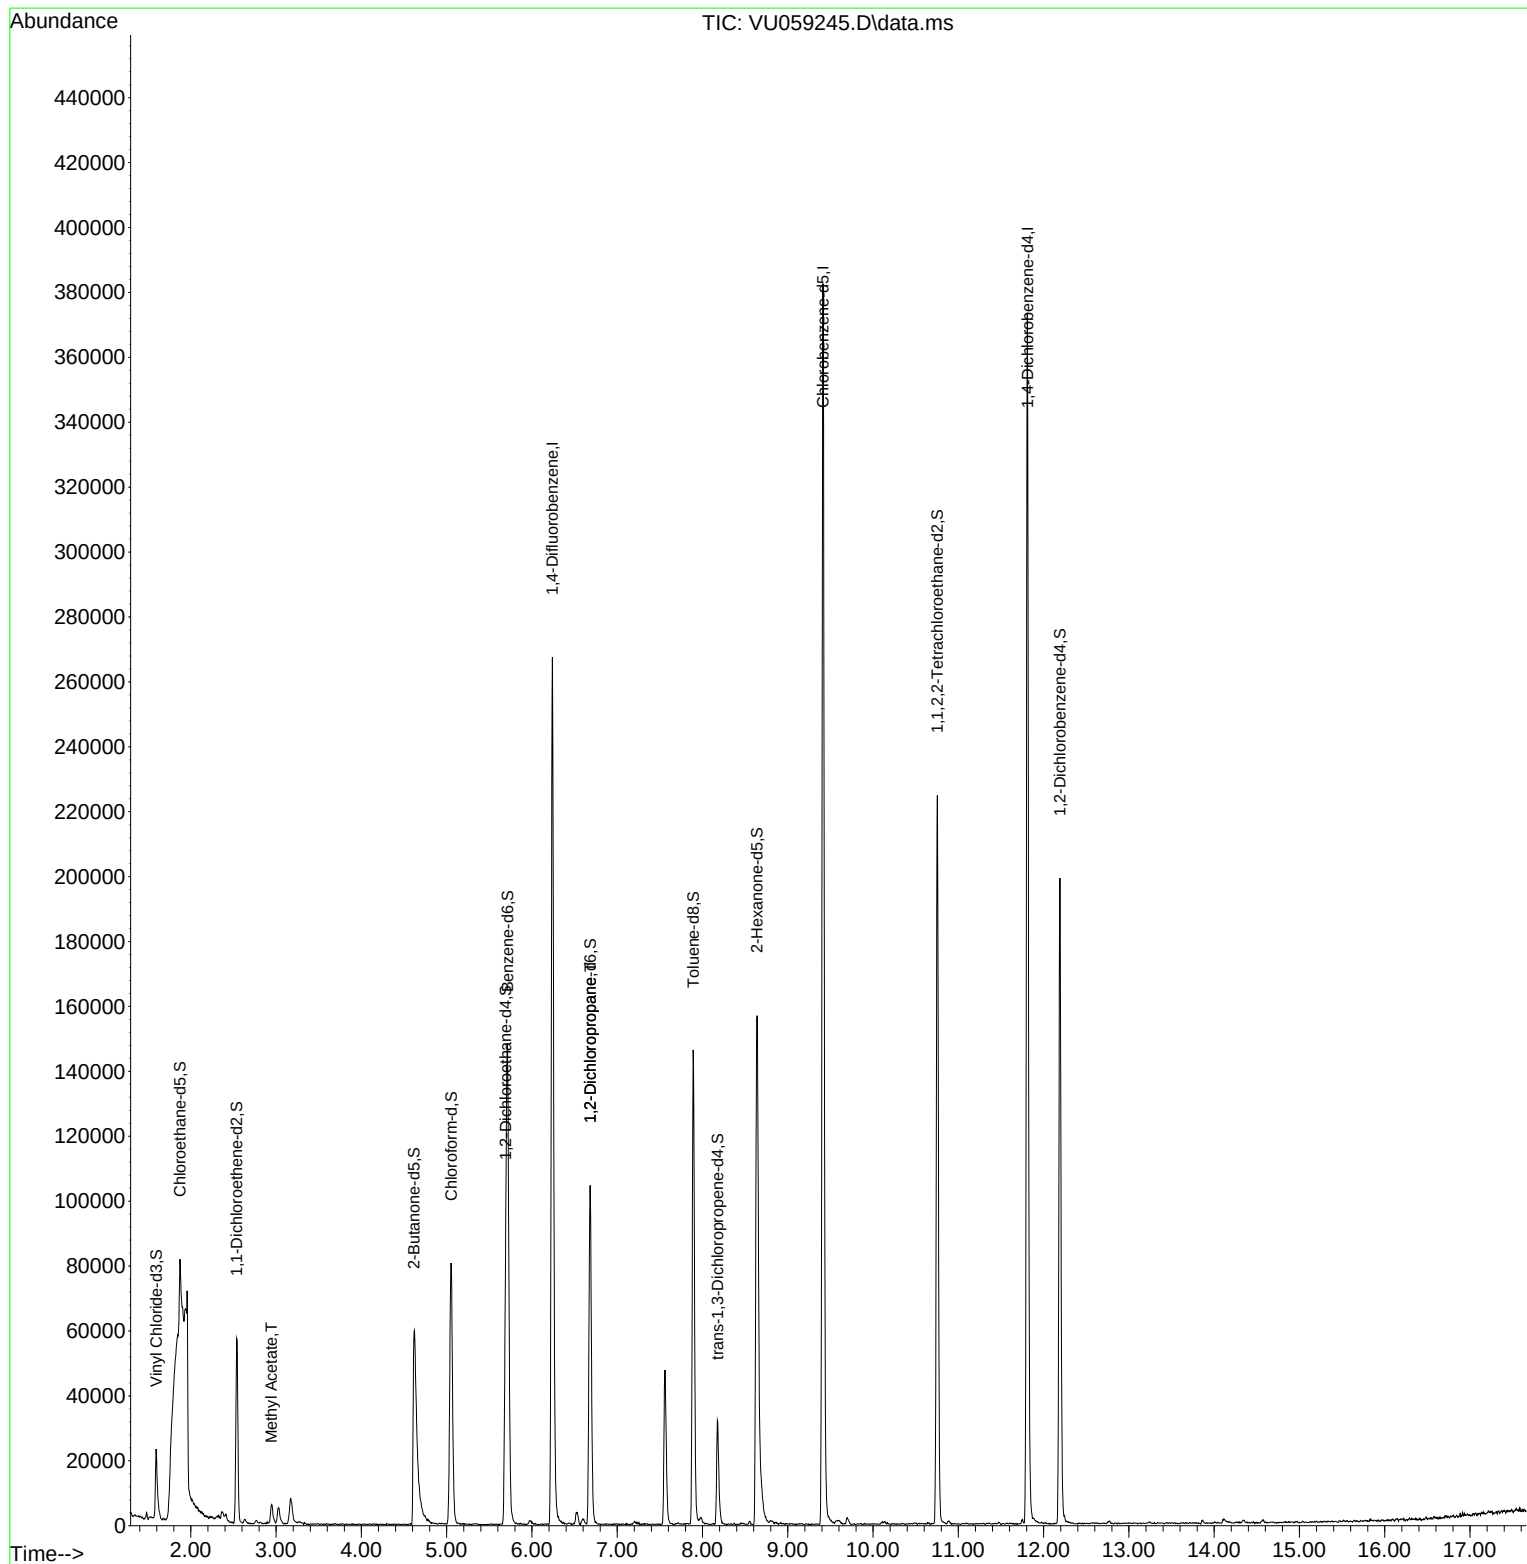


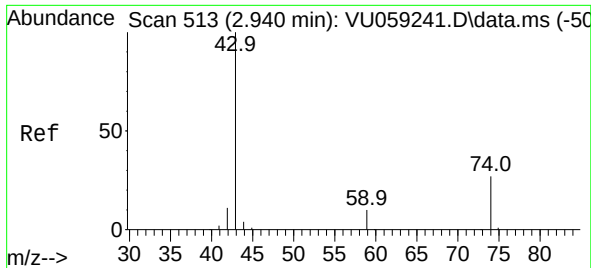

#15
Methyl Acetate
Concen: 3.743 ug/L
RT: 2.943 min Scan# 513
Delta R.T. 0.003 min
Lab File: VU059245.D
Acq: 14 Jun 2024 14:15

Instrument :
MSVOA_U
ClientSampleId :

Tgt Ion: 43 Resp: 8517
Ion Ratio Lower Upper
43 100
74 24.5 20.8 31.2

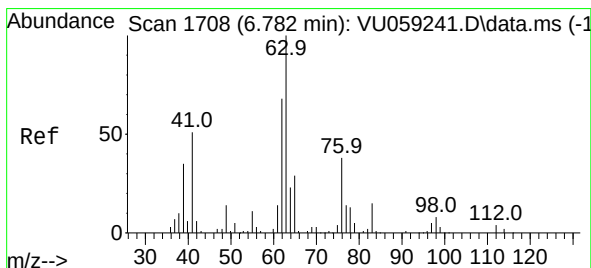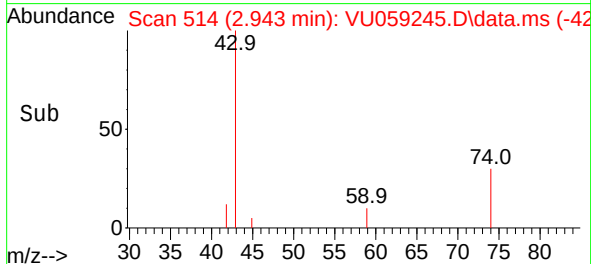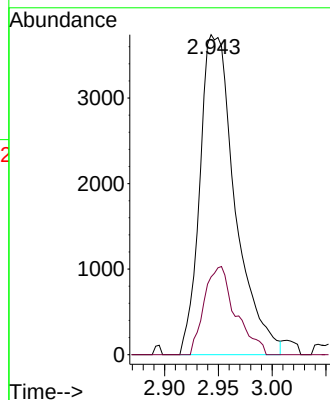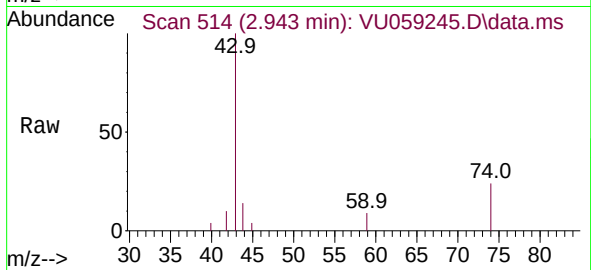

#37
1,2-Dichloropropane
Concen: 2.555 ug/L
RT: 6.683 min Scan# 1677
Delta R.T. -0.100 min
Lab File: VU059245.D
Acq: 14 Jun 2024 14:15

Tgt Ion: 63 Resp: 5808
Ion Ratio Lower Upper
63 100
112 0.0 2.6 4.0#

