

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061424\
 Data File : VU059247.D
 Acq On : 14 Jun 2024 15:00
 Operator : MD/SY
 Sample : P2775-12ME
 Misc : 6.11g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Jun 15 02:51:57 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 15 02:48:14 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.238	114	326616	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	334945	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	158707	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.592	65	43741	22.367	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	44.740%#		
7) Chloroethane-d5	1.872	69	38859	23.197	ug/L	-0.04
Spiked Amount 50.000	Range 70 - 130		Recovery =	46.400%#		
11) 1,1-Dichloroethene-d2	2.537	63	69171	17.920	ug/L	-0.03
Spiked Amount 50.000	Range 60 - 125		Recovery =	35.840%#		
21) 2-Butanone-d5	4.618	46	237892	129.060	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	129.060%		
24) Chloroform-d	5.049	84	159400	40.945	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	81.880%		
26) 1,2-Dichloroethane-d4	5.688	65	102809	43.087	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	86.180%		
32) Benzene-d6	5.714	84	268274	34.897	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	69.800%#		
36) 1,2-Dichloropropane-d6	6.682	67	108879	41.077	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	82.160%		
41) Toluene-d8	7.891	98	212392	32.546	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	65.100%#		
43) trans-1,3-Dichloroprop...	8.174	79	42067	39.262	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	78.520%		
47) 2-Hexanone-d5	8.637	63	150572	122.843	ug/L	0.01
Spiked Amount 100.000	Range 45 - 130		Recovery =	122.840%		
56) 1,1,2,2-Tetrachloroeth...	10.753	84	245436	54.712	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	109.420%		
66) 1,2-Dichlorobenzene-d4	12.190	152	113765	48.034	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	96.060%		
Target Compounds						Qvalue
15) Methyl Acetate	2.946	43	15460	4.505	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061424\
Data File : VU059247.D
Acq On : 14 Jun 2024 15:00
Operator : MD/SY
Sample : P2775-12ME
Misc : 6.11g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: Jun 15 02:51:57 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jun 15 02:48:14 2024
Response via : Initial Calibration

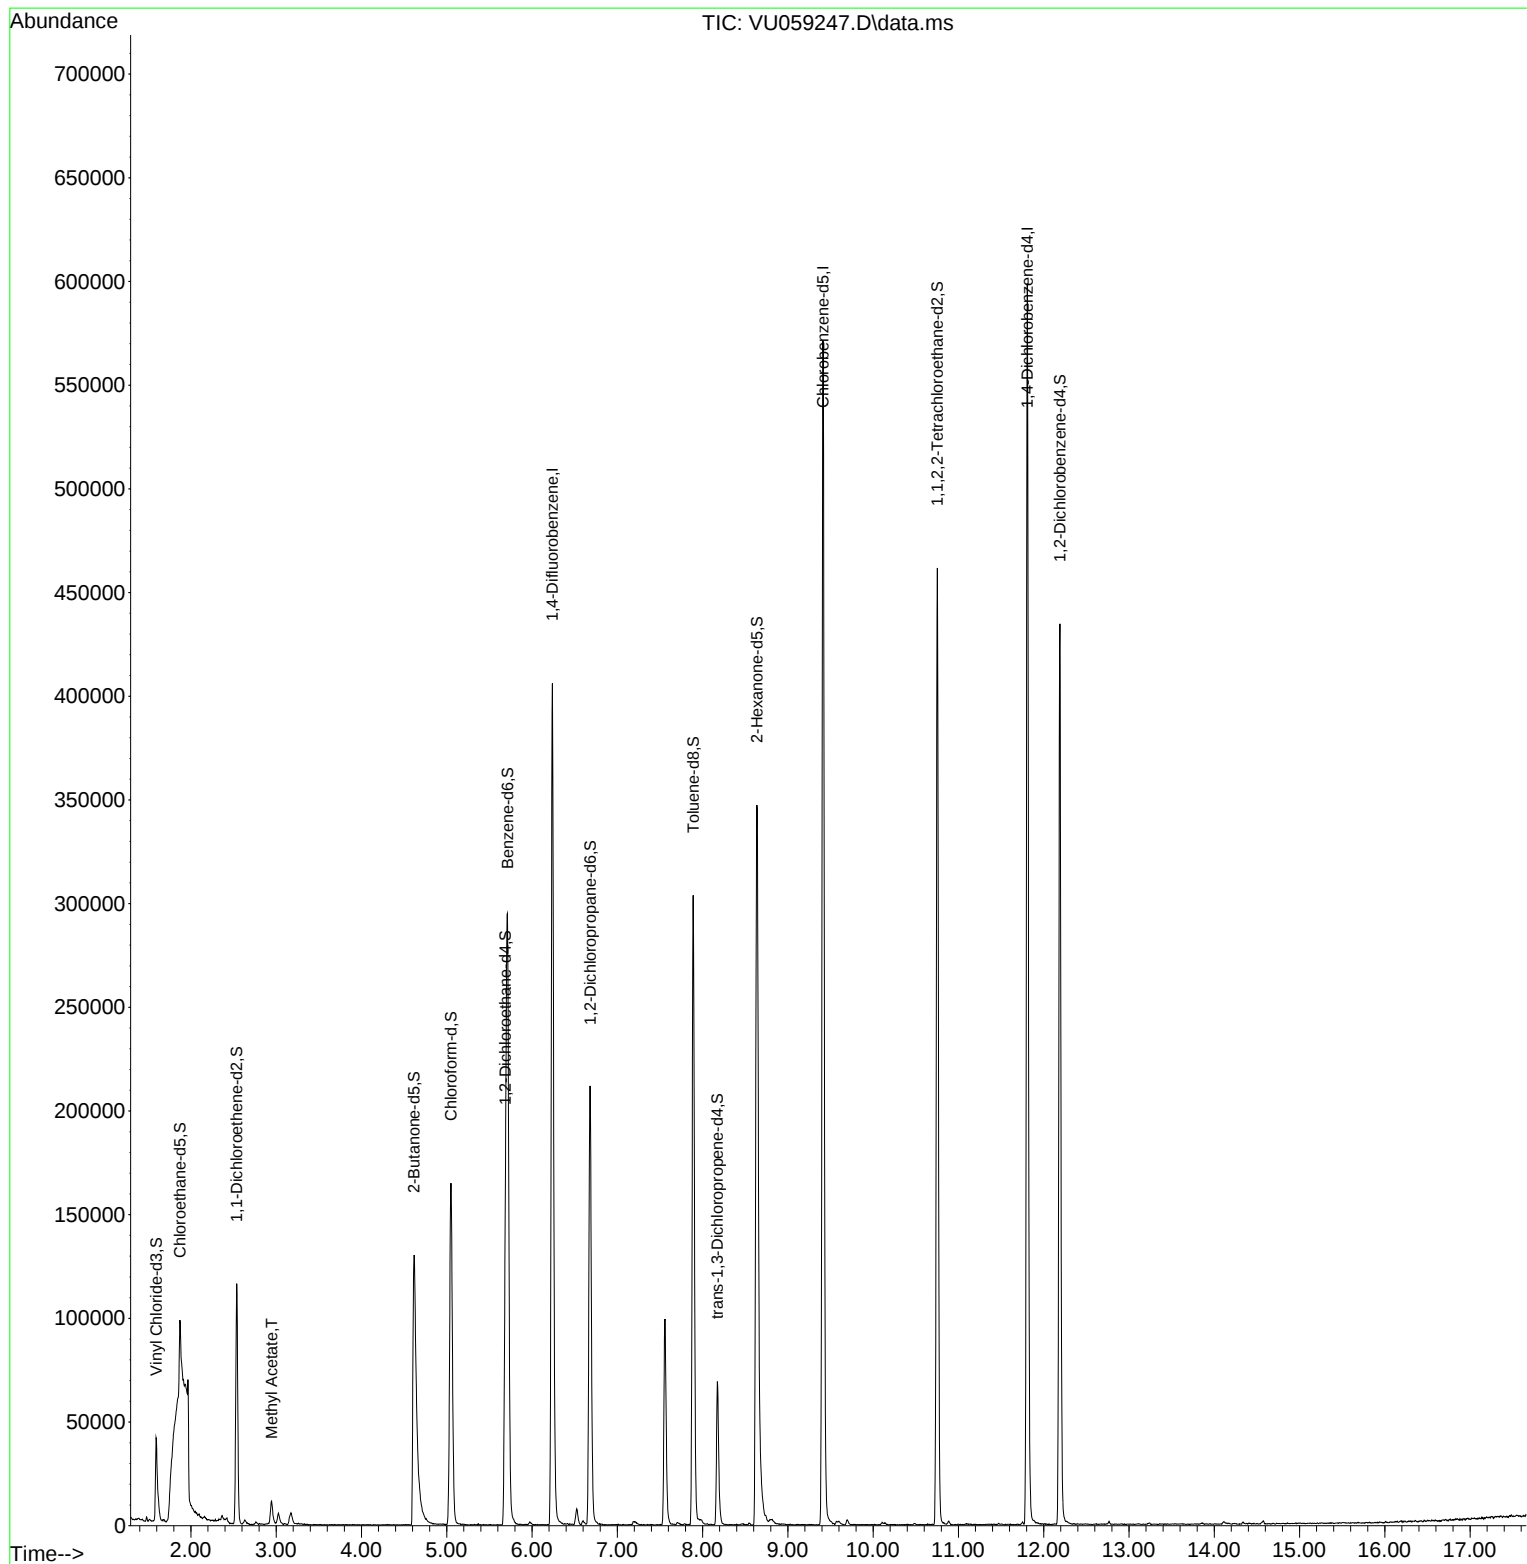

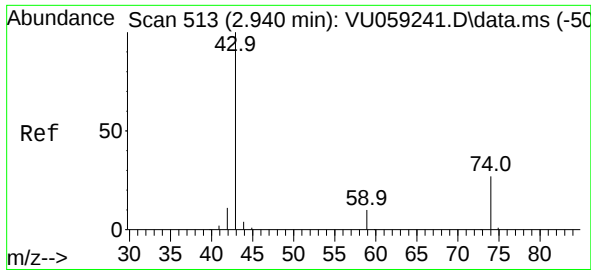

#15
Methyl Acetate
Concen: 4.505 ug/L
RT: 2.946 min Scan# 51
Delta R.T. 0.006 min
Lab File: VU059247.D
Acq: 14 Jun 2024 15:00

Instrument :
MSVOA_U
ClientSampleId :

Tgt Ion: 43 Resp: 15460
Ion Ratio Lower Upper
43 100
74 23.3 20.8 31.2

