

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061424\
 Data File : VU059243.D
 Acq On : 14 Jun 2024 13:31
 Operator : MD/SY
 Sample : VU0614WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK074

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M

Title : VOC Analysis

Signal : TIC: VU059243.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	111	rVB	90256	105238	14.78%	1.868%
2	1.760	140	146	156	rVB7	2802	4301	0.60%	0.076%
3	1.908	184	192	210	rVB	78585	106071	14.89%	1.883%
4	2.191	278	280	282	rBV2	569	219	0.03%	0.004%
5	2.252	296	299	301	rBV2	576	404	0.06%	0.007%
6	2.560	383	395	418	rVV	141613	234366	32.91%	4.160%
7	2.682	430	433	441	rVB2	416	482	0.07%	0.009%
8	2.789	457	466	475	rVB	1790	3016	0.42%	0.054%
9	2.898	497	500	502	rBV2	301	234	0.03%	0.004%
10	3.039	533	544	555	rVB3	3829	6928	0.97%	0.123%
11	3.171	575	585	588	rBV3	615	832	0.12%	0.015%
12	3.223	597	601	603	rBV2	236	222	0.03%	0.004%
13	3.348	633	640	652	rVB4	1406	2590	0.36%	0.046%
14	3.496	682	686	691	rBV2	258	296	0.04%	0.005%
15	4.139	881	886	891	rVB	328	369	0.05%	0.007%
16	4.171	891	896	899	rBV	290	299	0.04%	0.005%
17	4.219	908	911	918	rVB2	216	223	0.03%	0.004%
18	4.303	933	937	942	rBV2	162	206	0.03%	0.004%
19	4.477	987	991	995	rVB2	219	203	0.03%	0.004%
20	4.612	1024	1033	1069	rBV	67109	179146	25.15%	3.180%
21	4.808	1092	1094	1097	rVB2	389	213	0.03%	0.004%
22	5.052	1155	1170	1194	rBV	128598	285105	40.03%	5.061%
23	5.232	1221	1226	1229	rBV2	459	433	0.06%	0.008%
24	5.300	1244	1247	1250	rBV3	448	303	0.04%	0.005%
25	5.364	1264	1267	1269	rBV2	309	205	0.03%	0.004%
26	5.377	1269	1271	1277	rVB2	637	560	0.08%	0.010%
27	5.435	1285	1289	1295	rVB2	495	610	0.09%	0.011%
28	5.515	1311	1314	1318	rVV2	510	409	0.06%	0.007%
29	5.583	1330	1335	1337	rBV	268	278	0.04%	0.005%
30	5.634	1346	1351	1356	rBV2	350	475	0.07%	0.008%
31	5.718	1357	1377	1398	rBV2	262044	712228	100.00%	12.642%
32	5.898	1430	1433	1435	rVB3	357	201	0.03%	0.004%
33	6.055	1479	1482	1488	rVV3	253	269	0.04%	0.005%
34	6.142	1507	1509	1514	rVB3	369	309	0.04%	0.005%
35	6.168	1514	1517	1522	rBV2	222	246	0.03%	0.004%
36	6.242	1524	1540	1567	rBV	252300	494109	69.38%	8.770%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061424\
 Data File : VU059243.D
 Acq On : 14 Jun 2024 13:31
 Operator : MD/SY
 Sample : VU0614WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK074

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

37	6.528	1620	1629	1641	rBV8	5175	10711	1.50%	0.190%
38	6.682	1663	1677	1710	rBV	167182	329327	46.24%	5.846%
39	6.827	1720	1722	1728	rVB	341	295	0.04%	0.005%
40	6.962	1759	1764	1768	rBV2	369	340	0.05%	0.006%
41	6.988	1768	1772	1778	rVV	255	301	0.04%	0.005%
42	7.017	1778	1781	1787	rVB2	259	250	0.04%	0.004%
43	7.168	1823	1828	1830	rBV2	286	272	0.04%	0.005%
44	7.197	1830	1837	1848	rVB4	1510	2413	0.34%	0.043%
45	7.277	1855	1862	1868	rBV2	374	588	0.08%	0.010%
46	7.470	1919	1922	1928	rBV2	214	269	0.04%	0.005%
47	7.560	1939	1950	1974	rBV	75177	139017	19.52%	2.468%
48	7.669	1981	1984	1989	rVB2	300	253	0.04%	0.004%
49	7.698	1989	1993	1997	rBV4	726	840	0.12%	0.015%
50	7.772	2010	2016	2018	rBV	285	240	0.03%	0.004%
51	7.801	2018	2025	2030	rBV4	698	1111	0.16%	0.020%
52	7.891	2040	2053	2088	rBV	296244	529222	74.31%	9.394%
53	8.174	2131	2141	2164	rVV2	50595	93177	13.08%	1.654%
54	8.258	2164	2167	2172	rVB4	633	448	0.06%	0.008%
55	8.348	2191	2195	2199	rBV2	418	430	0.06%	0.008%
56	8.399	2206	2211	2215	rBV3	771	710	0.10%	0.013%
57	8.438	2220	2223	2225	rBV	277	221	0.03%	0.004%
58	8.499	2239	2242	2244	rBV2	245	199	0.03%	0.004%
59	8.547	2250	2257	2258	rBV3	1372	1235	0.17%	0.022%
60	8.628	2270	2282	2314	rBV	165983	349601	49.09%	6.205%
61	8.849	2348	2351	2355	rBV2	388	262	0.04%	0.005%
62	9.036	2405	2409	2413	rVB2	371	280	0.04%	0.005%
63	9.113	2430	2433	2440	rVB	360	400	0.06%	0.007%
64	9.412	2513	2526	2560	rBV	367877	630381	88.51%	11.189%
65	9.570	2570	2575	2585	rVB3	1923	2953	0.41%	0.052%
66	9.698	2606	2615	2621	rBV3	1347	2070	0.29%	0.037%
67	9.853	2660	2663	2670	rVB	369	405	0.06%	0.007%
68	9.898	2670	2677	2678	rBV2	230	257	0.04%	0.005%
69	10.103	2735	2741	2743	rBV3	762	912	0.13%	0.016%
70	10.126	2746	2748	2752	rVB2	871	531	0.07%	0.009%
71	10.290	2794	2799	2802	rVB2	443	394	0.06%	0.007%
72	10.328	2805	2811	2814	rBV2	343	383	0.05%	0.007%
73	10.415	2836	2838	2846	rVV	156	202	0.03%	0.004%
74	10.489	2855	2861	2869	rVB4	1054	1508	0.21%	0.027%
75	10.644	2903	2909	2911	rBV4	608	591	0.08%	0.010%
76	10.750	2928	2942	2960	rBV	225641	377879	53.06%	6.707%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061424\
 Data File : VU059243.D
 Acq On : 14 Jun 2024 13:31
 Operator : MD/SY
 Sample : VU0614WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK074

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

77	11.081	3041	3045	3047	rBV2	600	502	0.07%	0.009%
78	11.473	3164	3167	3176	rVB2	896	973	0.14%	0.017%
79	11.589	3199	3203	3208	rVB2	293	326	0.05%	0.006%
80	11.615	3208	3211	3215	rBV2	229	242	0.03%	0.004%
81	11.750	3245	3253	3260	rBV3	2276	3469	0.49%	0.062%
82	11.808	3260	3271	3289	rBV	320505	535016	75.12%	9.497%
83	11.978	3322	3324	3329	rVB3	357	237	0.03%	0.004%
84	12.036	3339	3342	3344	rBV2	314	238	0.03%	0.004%
85	12.187	3377	3389	3416	rBV	260756	449657	63.13%	7.981%
86	12.769	3567	3570	3578	rVB2	601	599	0.08%	0.011%
87	12.984	3632	3637	3641	rBV2	371	444	0.06%	0.008%
88	13.229	3706	3713	3726	rVB4	1588	2471	0.35%	0.044%
89	13.470	3786	3788	3794	rBV2	427	398	0.06%	0.007%
90	13.849	3899	3906	3917	rBV6	2180	4209	0.59%	0.075%
91	14.036	3960	3964	3966	rBV	340	216	0.03%	0.004%
92	14.100	3978	3984	3997	rBV3	3525	6281	0.88%	0.111%
93	14.306	4045	4048	4050	rBV	416	296	0.04%	0.005%
94	14.332	4050	4056	4064	rVV7	2529	3798	0.53%	0.067%
95	14.412	4079	4081	4084	rVV	424	240	0.03%	0.004%
96	14.515	4110	4113	4117	rBV2	402	312	0.04%	0.006%
97	14.579	4130	4133	4138	rBV2	290	278	0.04%	0.005%
98	14.637	4147	4151	4154	rBV2	428	386	0.05%	0.007%
99	16.103	4605	4607	4609	rBV2	595	383	0.05%	0.007%
100	16.171	4625	4628	4630	rBV2	553	328	0.05%	0.006%




Sum of corrected areas: 5633775

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061424\
Data File : VU059243.D
Acq On : 14 Jun 2024 13:31
Operator : MD/SY
Sample : VU0614WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK074

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

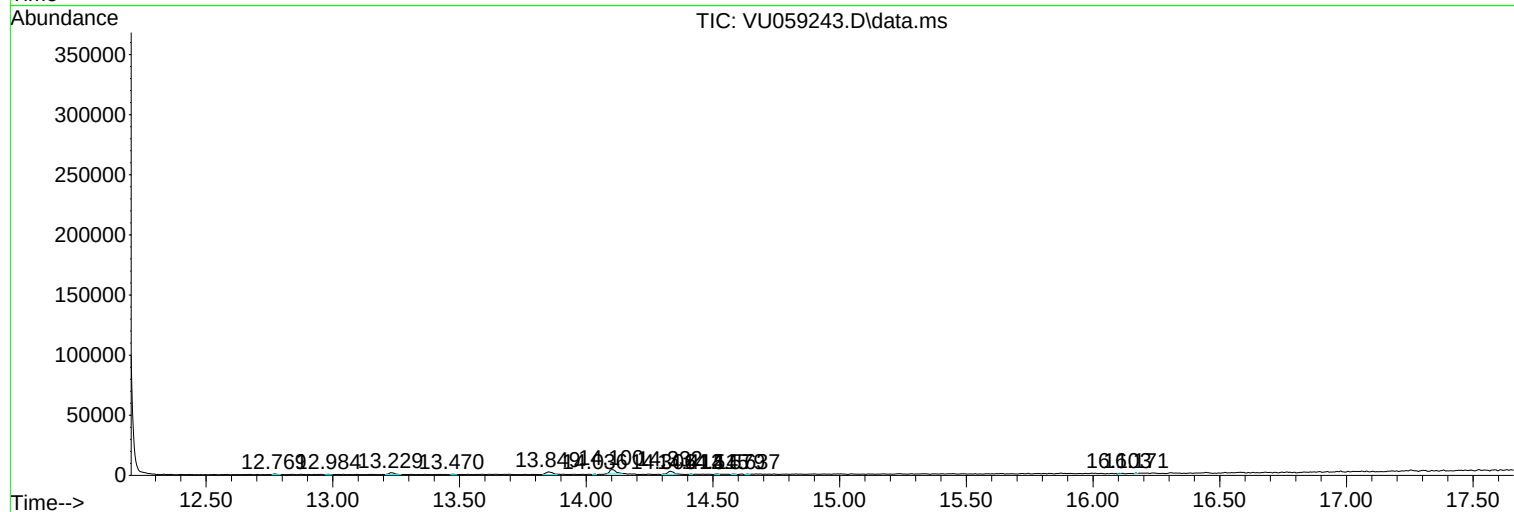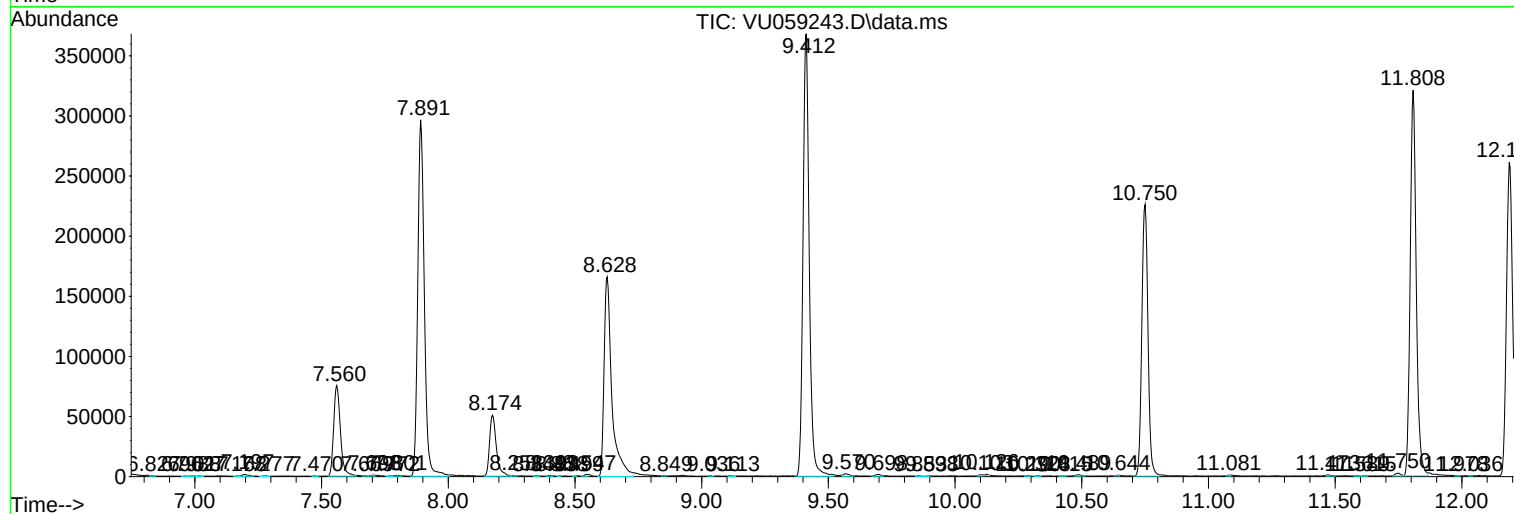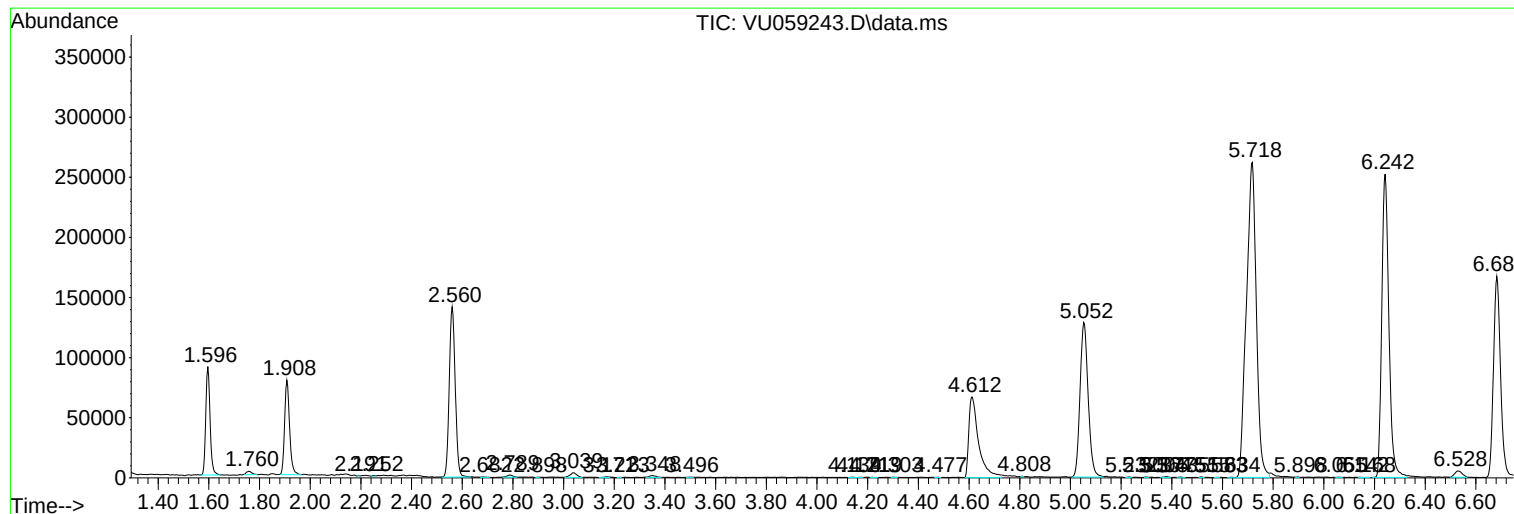

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061424\
Data File : VU059243.D
Acq On : 14 Jun 2024 13:31
Operator : MD/SY
Sample : VU0614WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK074

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061424\
Data File : VU059243.D
Acq On : 14 Jun 2024 13:31
Operator : MD/SY
Sample : VU0614WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK074

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc