

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061424\
 Data File : VU059258.D
 Acq On : 14 Jun 2024 19:16
 Operator : MD/SY
 Sample : P2844-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A4D82

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M

Title : VOC Analysis

Signal : TIC: VU059258.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	88	95	113	rVB	87726	102879	14.64%	1.833%
2	1.760	141	146	153	rBV2	3793	4717	0.67%	0.084%
3	1.907	184	192	207	rBV	75385	101946	14.50%	1.816%
4	2.264	300	303	311	rVB5	1262	1432	0.20%	0.026%
5	2.325	320	322	325	rBV3	676	358	0.05%	0.006%
6	2.493	370	374	379	rBV3	416	345	0.05%	0.006%
7	2.560	383	395	407	rVV	136025	221039	31.45%	3.937%
8	2.618	407	413	428	rVB	7004	12962	1.84%	0.231%
9	2.753	445	455	461	rBV3	627	1273	0.18%	0.023%
10	2.949	513	516	518	rBV2	364	293	0.04%	0.005%
11	3.039	532	544	554	rBV3	2995	5177	0.74%	0.092%
12	3.178	572	587	605	rBV	15495	36438	5.18%	0.649%
13	3.293	619	623	627	rBV2	205	250	0.04%	0.004%
14	3.399	653	656	661	rVB	287	211	0.03%	0.004%
15	3.731	754	759	762	rBV2	273	256	0.04%	0.005%
16	3.882	800	806	811	rBV	163	252	0.04%	0.004%
17	4.345	945	950	953	rVV2	184	211	0.03%	0.004%
18	4.438	973	979	983	rVB2	176	201	0.03%	0.004%
19	4.612	1018	1033	1059	rBV	78054	207977	29.59%	3.705%
20	4.994	1148	1152	1153	rBV	402	289	0.04%	0.005%
21	5.055	1156	1171	1197	rVV	125171	277808	39.52%	4.949%
22	5.184	1207	1211	1214	rBV3	233	233	0.03%	0.004%
23	5.293	1243	1245	1248	rBV	425	206	0.03%	0.004%
24	5.483	1302	1304	1309	rVB2	340	303	0.04%	0.005%
25	5.509	1309	1312	1315	rBV2	314	212	0.03%	0.004%
26	5.718	1356	1377	1399	rBV2	256524	702869	100.00%	12.520%
27	5.946	1446	1448	1455	rVB2	341	322	0.05%	0.006%
28	5.991	1459	1462	1467	rVV3	333	345	0.05%	0.006%
29	6.094	1491	1494	1500	rVB	287	258	0.04%	0.005%
30	6.129	1500	1505	1507	rBV3	404	385	0.05%	0.007%
31	6.242	1527	1540	1561	rBV	254208	491362	69.91%	8.753%
32	6.435	1596	1600	1604	rBV2	409	354	0.05%	0.006%
33	6.528	1620	1629	1642	rBV6	4941	9059	1.29%	0.161%
34	6.615	1651	1656	1662	rVB	246	254	0.04%	0.005%
35	6.682	1664	1677	1702	rBV	163300	321580	45.75%	5.728%
36	6.820	1717	1720	1724	rVB2	461	347	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061424\
 Data File : VU059258.D
 Acq On : 14 Jun 2024 19:16
 Operator : MD/SY
 Sample : P2844-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A4D82

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

37	7.007	1775	1778	1782	rVB2	353	308	0.04%	0.005%
38	7.126	1812	1815	1820	rVB2	243	264	0.04%	0.005%
39	7.190	1830	1835	1850	rVB4	1435	2794	0.40%	0.050%
40	7.438	1906	1912	1919	rBV2	348	478	0.07%	0.009%
41	7.489	1924	1928	1932	rBV	289	304	0.04%	0.005%
42	7.560	1939	1950	1971	rBV2	72873	132455	18.84%	2.359%
43	7.705	1986	1995	1996	rBV2	1003	942	0.13%	0.017%
44	7.753	2007	2010	2017	rVB4	629	518	0.07%	0.009%
45	7.801	2020	2025	2030	rBV3	269	394	0.06%	0.007%
46	7.894	2040	2054	2074	rBV	286286	509021	72.42%	9.067%
47	8.174	2131	2141	2165	rBV	49691	87580	12.46%	1.560%
48	8.393	2207	2209	2215	rVB2	481	430	0.06%	0.008%
49	8.431	2215	2221	2223	rBV2	514	537	0.08%	0.010%
50	8.467	2223	2232	2243	rVV3	2970	5364	0.76%	0.096%
51	8.550	2253	2258	2263	rVV4	805	864	0.12%	0.015%
52	8.573	2263	2265	2268	rVV	358	224	0.03%	0.004%
53	8.627	2271	2282	2322	rBV	161365	335322	47.71%	5.973%
54	8.788	2325	2332	2342	rVV5	5065	10078	1.43%	0.180%
55	8.840	2346	2348	2352	rVB4	887	697	0.10%	0.012%
56	9.412	2513	2526	2556	rBV	371404	638054	90.78%	11.366%
57	9.701	2611	2616	2620	rVB	528	424	0.06%	0.008%
58	9.888	2671	2674	2681	rVV2	261	205	0.03%	0.004%
59	9.917	2681	2683	2687	rVB	302	224	0.03%	0.004%
60	9.946	2687	2692	2694	rBV	270	264	0.04%	0.005%
61	10.177	2760	2764	2767	rVV	291	215	0.03%	0.004%
62	10.280	2792	2796	2801	rBV2	310	350	0.05%	0.006%
63	10.463	2851	2853	2860	rBV2	205	224	0.03%	0.004%
64	10.528	2870	2873	2879	rVB2	290	264	0.04%	0.005%
65	10.602	2892	2896	2898	rBV	243	227	0.03%	0.004%
66	10.750	2930	2942	2967	rVB	219819	362996	51.64%	6.466%
67	10.840	2967	2970	2973	rBV2	341	328	0.05%	0.006%
68	10.891	2974	2986	2994	rVV2	4236	7285	1.04%	0.130%
69	10.959	3004	3007	3013	rVB	278	260	0.04%	0.005%
70	10.987	3013	3016	3019	rBV2	329	279	0.04%	0.005%
71	11.065	3037	3040	3043	rVB2	426	295	0.04%	0.005%
72	11.386	3130	3140	3143	rBV2	355	539	0.08%	0.010%
73	11.450	3157	3160	3164	rBV3	300	231	0.03%	0.004%
74	11.502	3173	3176	3179	rVB	432	302	0.04%	0.005%
75	11.807	3259	3271	3297	rBV	329065	554052	78.83%	9.869%
76	12.087	3348	3358	3361	rBV5	1092	1424	0.20%	0.025%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061424\
Data File : VU059258.D
Acq On : 14 Jun 2024 19:16
Operator : MD/SY
Sample : P2844-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A4D82

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Title : VOC Analysis

77	12.187	3377	3389	3415	rBV	251154	435199	61.92%	7.752%
78	12.328	3429	3433	3436	rVB4	561	528	0.08%	0.009%
79	12.360	3440	3443	3445	rBV2	339	267	0.04%	0.005%
80	12.534	3491	3497	3506	rBV5	2208	3468	0.49%	0.062%
81	12.656	3532	3535	3538	rBV	287	219	0.03%	0.004%
82	12.766	3561	3569	3579	rBV3	2601	4437	0.63%	0.079%
83	12.897	3607	3610	3614	rBV2	260	250	0.04%	0.004%
84	13.235	3711	3715	3717	rBV2	396	294	0.04%	0.005%
85	13.402	3764	3767	3774	rVB2	294	317	0.05%	0.006%
86	13.557	3811	3815	3820	rVB2	274	302	0.04%	0.005%
87	13.585	3821	3824	3828	rBV	285	253	0.04%	0.005%
88	14.299	4042	4046	4049	rBV3	312	306	0.04%	0.005%
89	14.402	4075	4078	4084	rBV3	333	353	0.05%	0.006%
90	14.450	4090	4093	4095	rBV	347	274	0.04%	0.005%
91	14.569	4126	4130	4133	rBV3	558	583	0.08%	0.010%
92	14.888	4224	4229	4231	rBV2	447	455	0.06%	0.008%
93	14.952	4245	4249	4252	rBV3	445	448	0.06%	0.008%
94	14.984	4253	4259	4263	rVB5	1276	1439	0.20%	0.026%
95	15.097	4292	4294	4300	rVB2	382	281	0.04%	0.005%
96	15.637	4459	4462	4466	rVB2	428	318	0.05%	0.006%
97	15.820	4515	4519	4521	rBV	566	414	0.06%	0.007%
98	16.196	4634	4636	4639	rVB3	853	431	0.06%	0.008%
99	16.222	4639	4644	4649	rBV4	627	919	0.13%	0.016%
100	16.373	4688	4691	4695	rBV3	851	758	0.11%	0.014%




Sum of corrected areas: 5613932

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061424\
Data File : VU059258.D
Acq On : 14 Jun 2024 19:16
Operator : MD/SY
Sample : P2844-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A4D82

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

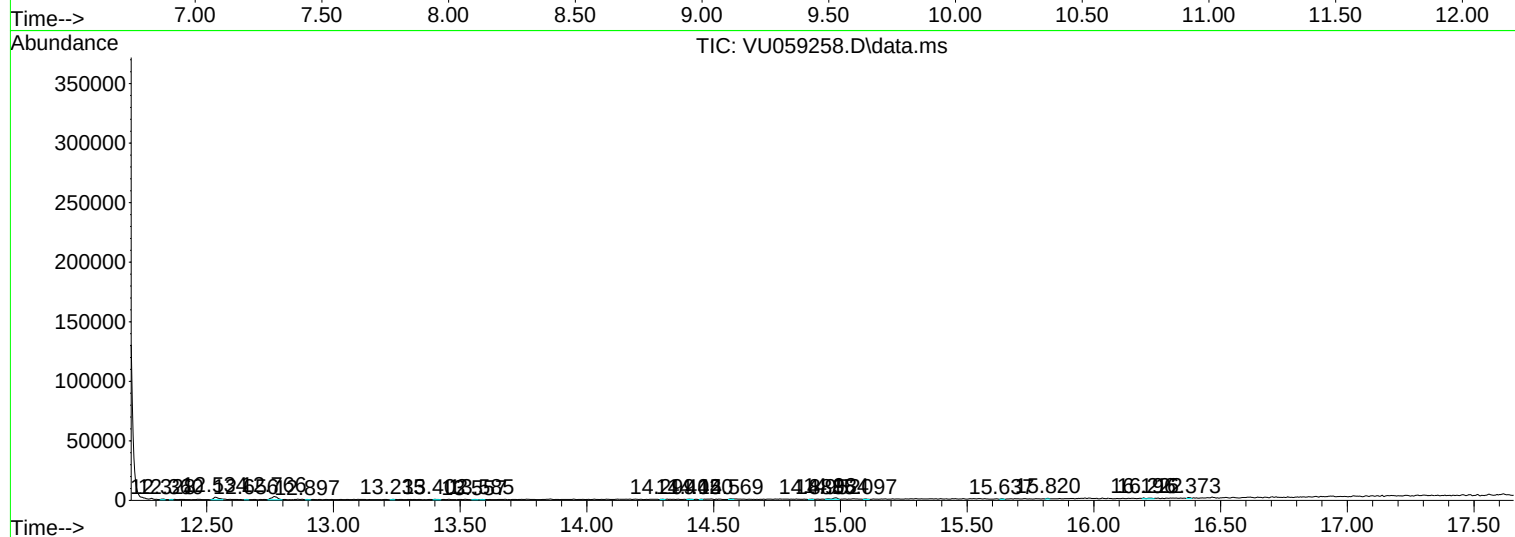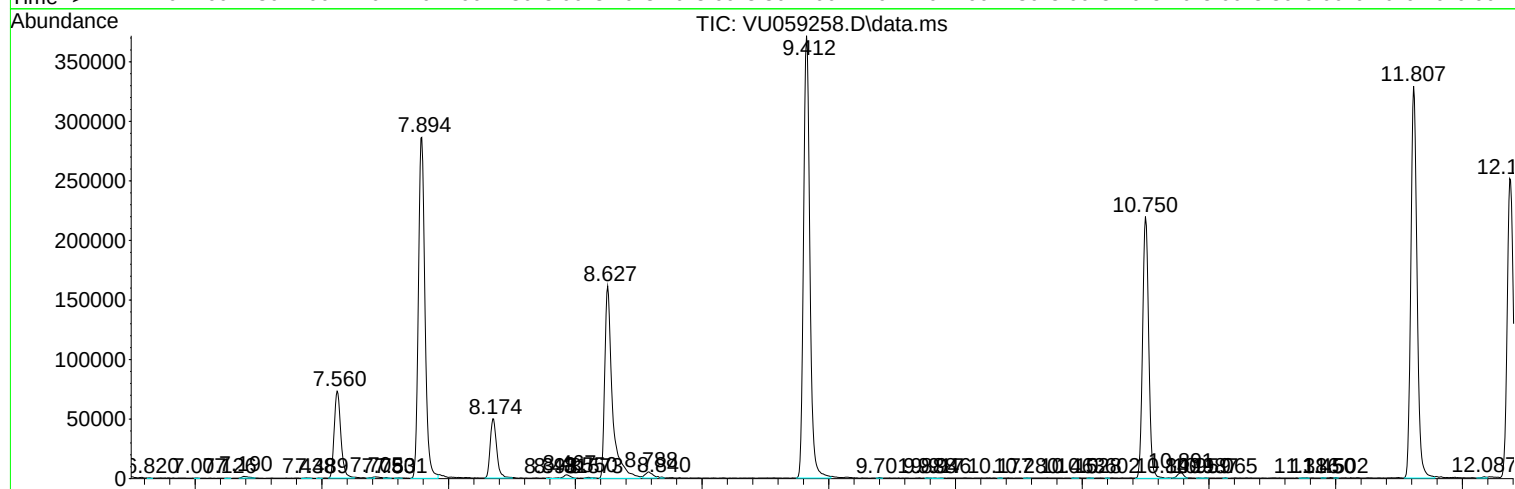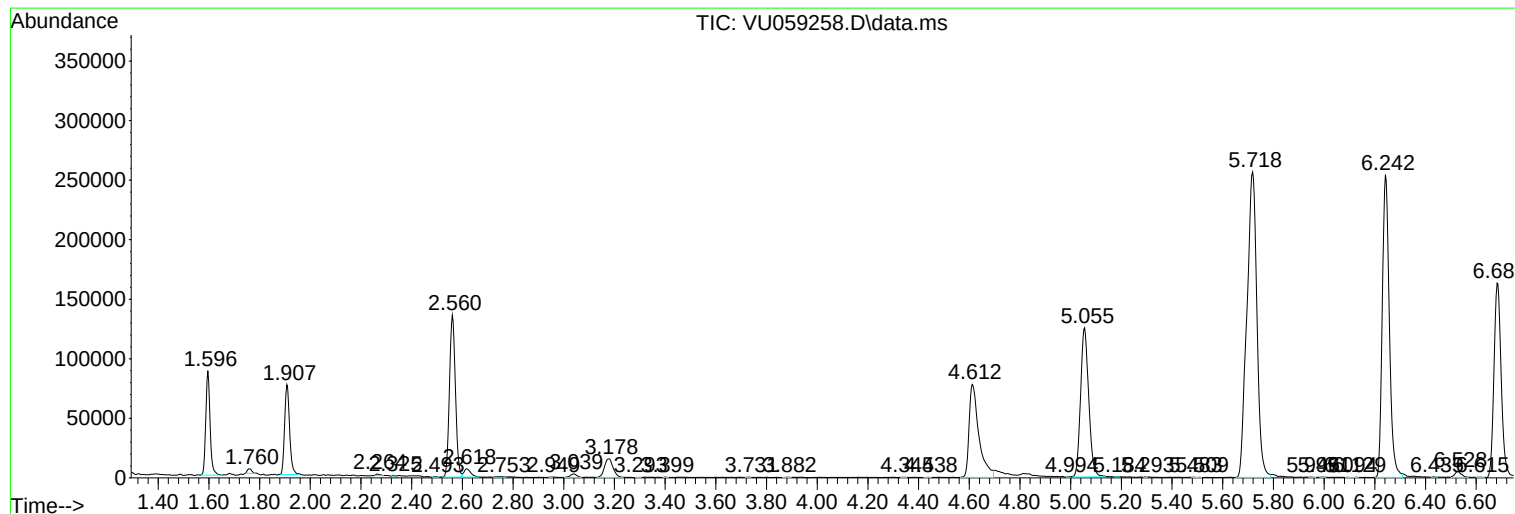

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061424\
Data File : VU059258.D
Acq On : 14 Jun 2024 19:16
Operator : MD/SY
Sample : P2844-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A4D82

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061424\
Data File : VU059258.D
Acq On : 14 Jun 2024 19:16
Operator : MD/SY
Sample : P2844-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A4D82

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------