

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061424\
 Data File : VU059259.D
 Acq On : 14 Jun 2024 19:39
 Operator : MD/SY
 Sample : P2844-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A4DD3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M

Title : VOC Analysis

Signal : TIC: VU059259.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	88	95	111	rVB	87914	103477	14.76%	1.860%
2	1.679	117	121	128	rVB3	1334	1525	0.22%	0.027%
3	1.760	138	146	151	rBV3	4159	6684	0.95%	0.120%
4	1.907	184	192	211	rVB	73106	102356	14.60%	1.840%
5	2.502	374	377	378	rBV	278	161	0.02%	0.003%
6	2.560	383	395	407	rBV	137016	222921	31.80%	4.007%
7	2.618	408	413	425	rVB	8168	13335	1.90%	0.240%
8	2.718	442	444	450	rBV2	253	194	0.03%	0.003%
9	3.039	534	544	554	rBV3	3618	6523	0.93%	0.117%
10	3.174	576	586	603	rVB4	2558	5864	0.84%	0.105%
11	3.245	603	608	614	rVB2	491	559	0.08%	0.010%
12	3.284	614	620	622	rBV	387	419	0.06%	0.008%
13	3.393	649	654	658	rVB2	169	166	0.02%	0.003%
14	3.422	658	663	667	rBV	195	228	0.03%	0.004%
15	3.550	700	703	708	rVB2	308	292	0.04%	0.005%
16	3.576	708	711	713	rBV	343	246	0.04%	0.004%
17	3.821	783	787	789	rBV	200	158	0.02%	0.003%
18	4.081	866	868	873	rVB2	264	223	0.03%	0.004%
19	4.120	873	880	884	rBV2	308	391	0.06%	0.007%
20	4.255	915	922	925	rVB	274	319	0.05%	0.006%
21	4.615	1022	1034	1063	rBV	66753	175679	25.06%	3.158%
22	4.923	1127	1130	1132	rBV2	494	261	0.04%	0.005%
23	4.962	1140	1142	1145	rBV	260	165	0.02%	0.003%
24	5.055	1155	1171	1194	rBV	125728	281568	40.17%	5.062%
25	5.190	1209	1213	1217	rVB2	372	288	0.04%	0.005%
26	5.374	1265	1270	1272	rBV2	299	268	0.04%	0.005%
27	5.718	1357	1377	1408	rBV2	254506	700925	100.00%	12.600%
28	5.859	1419	1421	1426	rVB2	548	404	0.06%	0.007%
29	6.097	1491	1495	1498	rVB3	225	179	0.03%	0.003%
30	6.187	1518	1523	1526	rVB2	192	209	0.03%	0.004%
31	6.242	1526	1540	1567	rBV	247650	486227	69.37%	8.741%
32	6.412	1590	1593	1598	rVB3	330	277	0.04%	0.005%
33	6.525	1620	1628	1640	rVV7	4602	8890	1.27%	0.160%
34	6.631	1659	1661	1664	rVB	321	182	0.03%	0.003%
35	6.682	1664	1677	1702	rBV	160068	319798	45.63%	5.749%
36	6.817	1718	1719	1723	rVB3	449	178	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061424\
 Data File : VU059259.D
 Acq On : 14 Jun 2024 19:39
 Operator : MD/SY
 Sample : P2844-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A4DD3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

37	6.843	1723	1727	1734	rVB2	321	419	0.06%	0.008%
38	7.161	1822	1826	1828	rBV2	368	321	0.05%	0.006%
39	7.197	1831	1837	1841	rBV3	1395	1793	0.26%	0.032%
40	7.409	1901	1903	1908	rBV2	202	241	0.03%	0.004%
41	7.560	1937	1950	1968	rBV2	72676	134160	19.14%	2.412%
42	7.705	1992	1995	1997	rVV3	503	264	0.04%	0.005%
43	7.746	2005	2008	2012	rVB3	440	280	0.04%	0.005%
44	7.795	2020	2023	2028	rVB2	414	440	0.06%	0.008%
45	7.824	2028	2032	2037	rBV2	338	411	0.06%	0.007%
46	7.891	2041	2053	2075	rBV	285780	507494	72.40%	9.123%
47	8.174	2132	2141	2167	rVV	50114	87872	12.54%	1.580%
48	8.345	2190	2194	2197	rVB	263	223	0.03%	0.004%
49	8.367	2197	2201	2204	rVB	342	298	0.04%	0.005%
50	8.399	2204	2211	2213	rBV	329	402	0.06%	0.007%
51	8.467	2221	2232	2246	rBV4	5168	9566	1.36%	0.172%
52	8.550	2253	2258	2264	rBV4	750	834	0.12%	0.015%
53	8.627	2271	2282	2320	rBV2	158743	334635	47.74%	6.016%
54	9.010	2398	2401	2407	rBV2	315	331	0.05%	0.006%
55	9.200	2456	2460	2466	rBV2	175	209	0.03%	0.004%
56	9.312	2492	2495	2500	rVV2	183	185	0.03%	0.003%
57	9.412	2513	2526	2552	rBV	370314	631516	90.10%	11.353%
58	9.566	2572	2574	2577	rBV3	392	159	0.02%	0.003%
59	9.666	2602	2605	2608	rBV	298	261	0.04%	0.005%
60	9.689	2610	2612	2616	rVB2	392	302	0.04%	0.005%
61	9.833	2653	2657	2658	rBV	241	182	0.03%	0.003%
62	9.978	2699	2702	2705	rVB	275	174	0.02%	0.003%
63	10.000	2705	2709	2713	rBV	249	264	0.04%	0.005%
64	10.110	2738	2743	2748	rVB3	311	344	0.05%	0.006%
65	10.254	2785	2788	2792	rVB2	251	210	0.03%	0.004%
66	10.274	2792	2794	2799	rVB	315	219	0.03%	0.004%
67	10.299	2799	2802	2806	rBV2	472	330	0.05%	0.006%
68	10.357	2817	2820	2824	rBV	194	185	0.03%	0.003%
69	10.750	2929	2942	2958	rBV	227347	365896	52.20%	6.578%
70	10.888	2974	2985	2996	rVB	9131	14807	2.11%	0.266%
71	10.997	3016	3019	3022	rVB2	248	174	0.02%	0.003%
72	11.132	3058	3061	3064	rBV	311	207	0.03%	0.004%
73	11.332	3120	3123	3126	rVB2	259	166	0.02%	0.003%
74	11.467	3161	3165	3171	rBV3	431	459	0.07%	0.008%
75	11.489	3171	3172	3175	rVV2	367	232	0.03%	0.004%
76	11.505	3175	3177	3185	rVB3	468	420	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061424\
 Data File : VU059259.D
 Acq On : 14 Jun 2024 19:39
 Operator : MD/SY
 Sample : P2844-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A4DD3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

77	11.807	3259	3271	3295	rBV	335808	552205	78.78%	9.927%
78	12.039	3339	3343	3345	rBV2	385	348	0.05%	0.006%
79	12.084	3353	3357	3358	rBV	937	648	0.09%	0.012%
80	12.116	3364	3367	3371	rBV5	728	445	0.06%	0.008%
81	12.187	3377	3389	3413	rBV	261368	445742	63.59%	8.013%
82	12.335	3432	3435	3441	rVB3	498	514	0.07%	0.009%
83	12.360	3441	3443	3447	rBV2	234	171	0.02%	0.003%
84	12.534	3488	3497	3508	rBV5	5040	8074	1.15%	0.145%
85	12.640	3527	3530	3534	rBV2	222	190	0.03%	0.003%
86	12.766	3559	3569	3585	rVB2	4527	7960	1.14%	0.143%
87	12.852	3590	3596	3606	rVB4	935	1391	0.20%	0.025%
88	12.913	3613	3615	3619	rBV3	286	241	0.03%	0.004%
89	13.000	3638	3642	3645	rBV2	321	313	0.04%	0.006%
90	13.103	3671	3674	3676	rBV2	211	166	0.02%	0.003%
91	13.839	3900	3903	3907	rBV2	290	261	0.04%	0.005%
92	14.177	4005	4008	4010	rBV	354	168	0.02%	0.003%
93	14.409	4076	4080	4085	rBV2	361	412	0.06%	0.007%
94	14.563	4125	4128	4129	rBV	383	205	0.03%	0.004%
95	14.643	4150	4153	4156	rBV2	388	261	0.04%	0.005%
96	14.843	4210	4215	4220	rBV3	348	451	0.06%	0.008%
97	14.978	4251	4257	4271	rVB5	2000	2938	0.42%	0.053%
98	15.251	4337	4342	4346	rBV	411	429	0.06%	0.008%
99	15.315	4358	4362	4364	rBV2	401	319	0.05%	0.006%
100	16.351	4681	4684	4686	rBV2	778	448	0.06%	0.008%




Sum of corrected areas: 5562724

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061424\
Data File : VU059259.D
Acq On : 14 Jun 2024 19:39
Operator : MD/SY
Sample : P2844-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A4DD3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

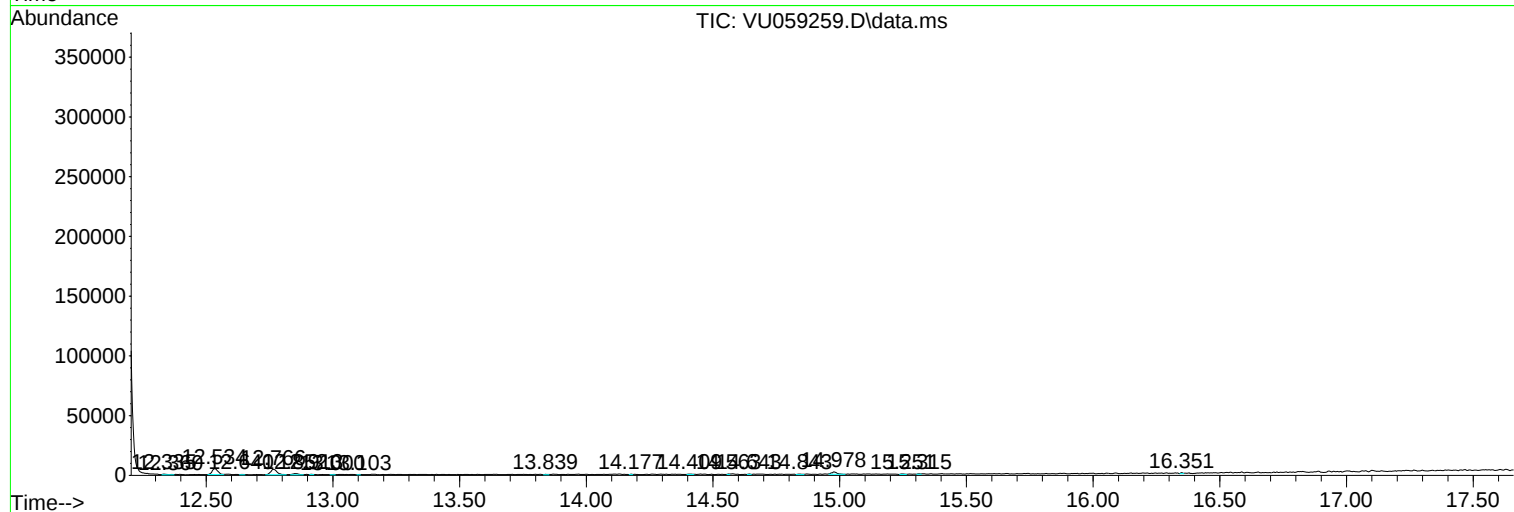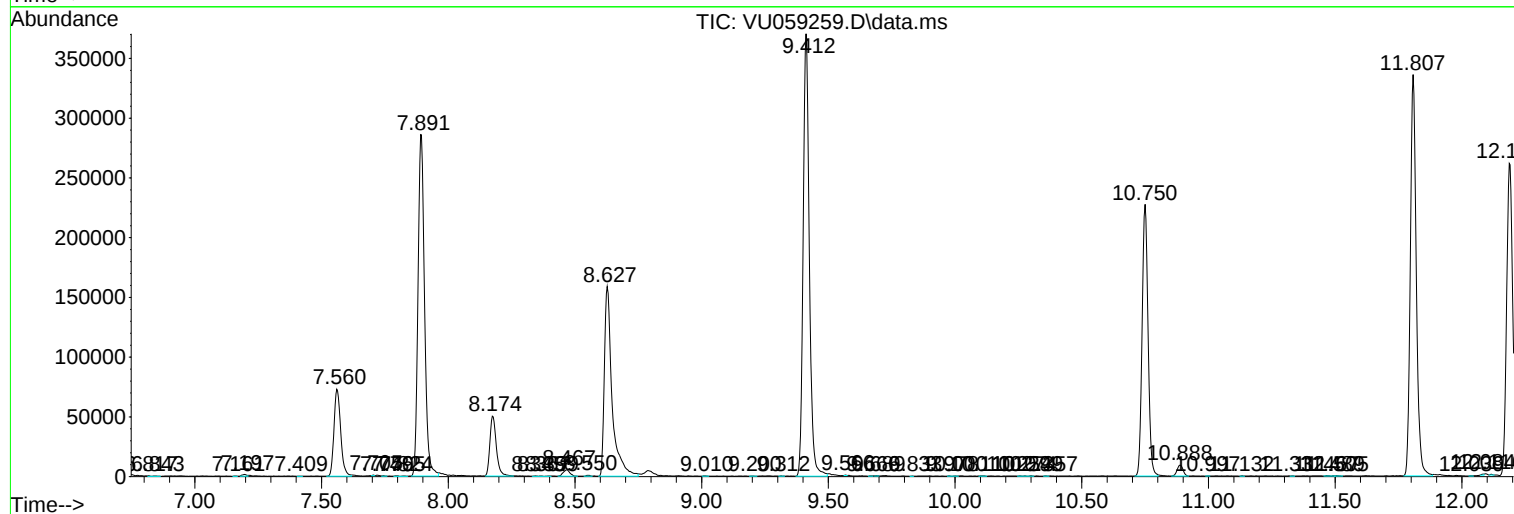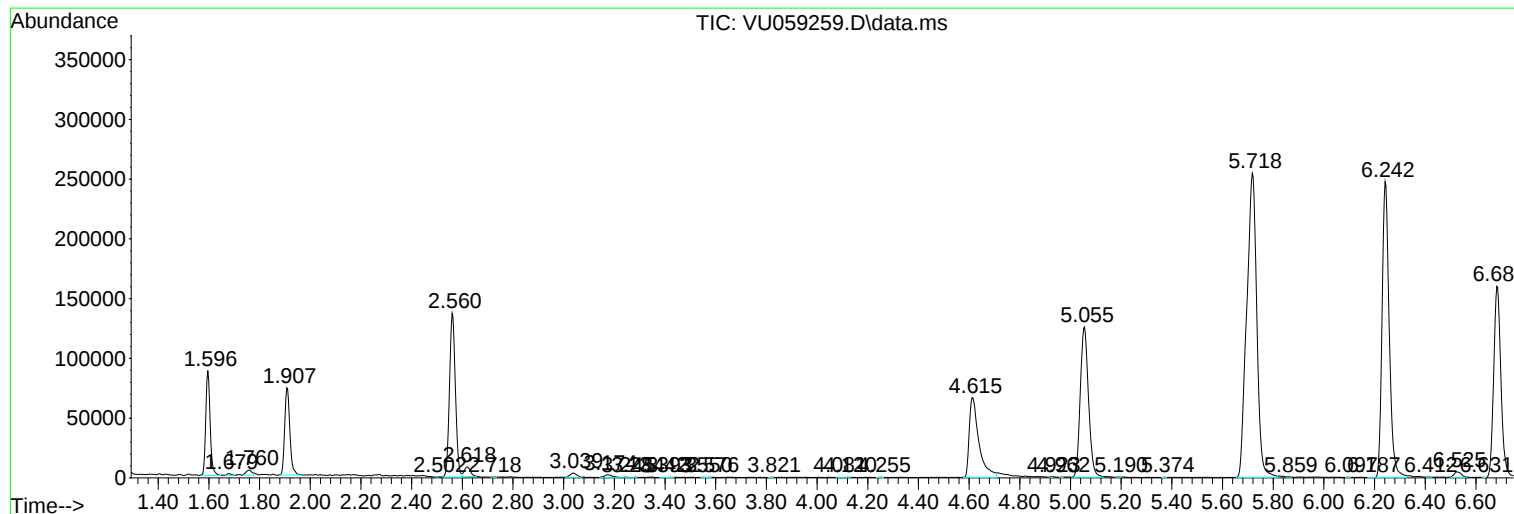

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061424\
Data File : VU059259.D
Acq On : 14 Jun 2024 19:39
Operator : MD/SY
Sample : P2844-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A4DD3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061424\
Data File : VU059259.D
Acq On : 14 Jun 2024 19:39
Operator : MD/SY
Sample : P2844-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A4DD3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------