
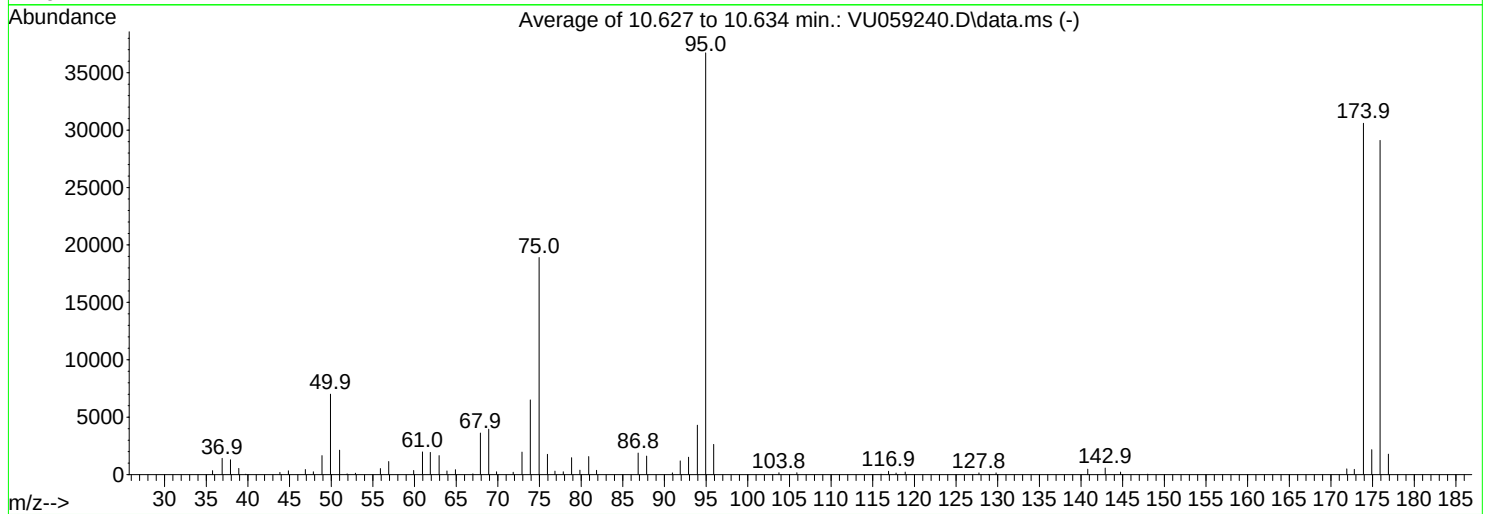


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061424\
Data File : VU059240.D
Acq On : 14 Jun 2024 11:59
Operator : MD/SY
Sample : BFB063
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB063

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Title : VOC Analysis
Last Update : Sat Jun 15 02:48:14 2024

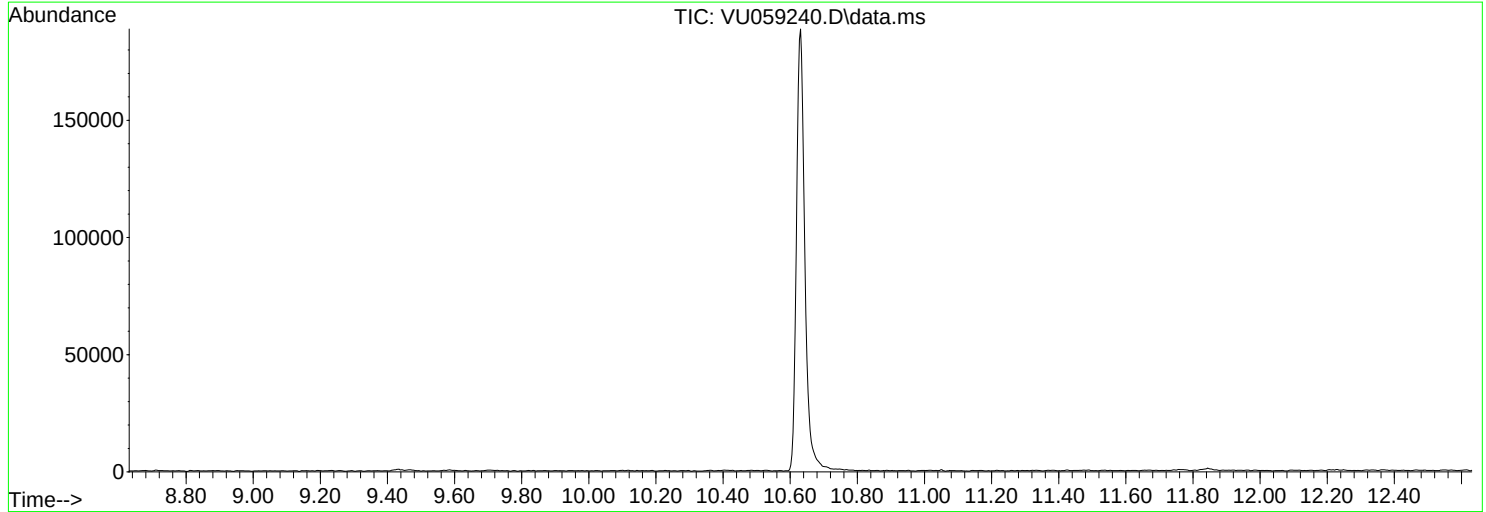

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2893

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.1	7004	PASS
75	95	30	80	51.5	18901	PASS
95	95	100	100	100.0	36728	PASS
96	95	5	9	7.2	2633	PASS
173	174	0.00	2	1.5	465	PASS
174	95	50	120	83.3	30597	PASS
175	174	5	9	7.1	2174	PASS
176	174	95	101	95.1	29107	PASS
177	176	5	9	6.1	1782	PASS

m/z	Abundance
39.70	132.0
43.80	359.0

Instrument :
MSVOA_U
ClientSampleId :
BFB063

m/z	Abundance
35.90	356.0
36.90	1515.0
37.90	1349.0
38.90	523.0
39.90	166.0
43.90	581.0
44.90	412.0
46.90	429.0
47.90	296.0
48.90	1765.0
49.90	6849.0
51.00	2322.0
51.90	119.0
52.90	113.0
55.90	544.0
56.90	1234.0
59.90	382.0
60.90	2064.0
61.90	1999.0
63.00	1781.0
63.90	342.0
64.90	445.0
67.90	3699.0
68.90	4082.0
69.90	290.0
71.90	177.0
72.90	2109.0
73.90	6623.0
74.90	18880.0
75.90	1898.0
76.90	320.0
77.90	220.0
78.90	1486.0
79.90	384.0
80.90	1571.0
81.90	380.0
86.90	1813.0
87.90	1762.0
90.90	162.0
91.90	1136.0
92.90	1397.0
94.00	4247.0
95.00	36744.0
95.90	2707.0
103.90	139.0
105.90	196.0
116.90	273.0
117.90	168.0
118.90	237.0
127.90	153.0
129.90	177.0
140.90	430.0
142.90	605.0
144.70	198.0
171.90	446.0
172.90	446.0
173.90	30240.0
174.90	2362.0
175.90	28760.0
176.90	1821.0

Instrument :
MSVOA_U
ClientSampleId :
BFB063

m/z	Abundance
35.70	354.0
36.90	1445.0
37.90	1345.0
38.90	530.0
39.80	174.0
44.00	564.0
44.90	325.0
46.90	451.0
47.90	265.0
48.90	1705.0
49.90	7197.0
51.00	2203.0
51.90	107.0
52.90	146.0
55.90	532.0
56.90	1158.0
59.90	357.0
61.00	2044.0
61.90	1968.0
62.90	1732.0
63.90	348.0
64.90	434.0
67.00	102.0
67.90	3716.0
68.90	4052.0
69.80	241.0
71.90	208.0
72.90	2055.0
73.90	6701.0
74.90	19512.0
76.00	1868.0
76.90	320.0
77.80	256.0
78.90	1485.0
79.90	403.0
80.90	1610.0
81.90	409.0
86.90	1946.0
87.90	1681.0
91.00	161.0
91.90	1262.0
92.90	1585.0
93.90	4463.0
95.00	37800.0
95.90	2688.0
103.70	187.0
105.90	175.0
116.90	297.0
117.80	139.0
118.90	237.0
127.70	168.0
129.80	152.0
140.80	496.0
142.90	600.0
144.80	226.0
171.90	511.0
172.80	477.0
173.90	31320.0
174.90	2254.0
175.90	29952.0
176.90	1824.0

Instrument :
MSVOA_U
ClientSampleId :
BFB063

m/z	Abundance
35.70	332.0
36.90	1298.0
37.90	1216.0
38.90	568.0
39.90	188.0
44.00	517.0
44.90	260.0
46.90	439.0
47.90	213.0
48.90	1502.0
49.90	6965.0
51.00	1891.0
52.90	128.0
55.90	509.0
56.90	1030.0
59.90	369.0
61.00	1819.0
61.90	1829.0
62.90	1481.0
63.90	292.0
64.90	399.0
67.00	110.0
67.90	3441.0
68.90	3748.0
69.80	224.0
71.80	228.0
72.90	1720.0
73.90	6206.0
75.00	18312.0
76.00	1541.0
76.90	285.0
77.80	270.0
78.90	1462.0
79.80	389.0
80.90	1527.0
81.80	353.0
86.80	1908.0
87.80	1412.0
91.00	160.0
91.90	1203.0
92.90	1594.0
93.90	4210.0
94.90	35640.0
95.90	2504.0
103.70	193.0
105.90	142.0
116.00	131.0
116.90	306.0
117.80	133.0
118.90	203.0
127.70	146.0
128.90	104.0
129.80	133.0
140.80	506.0
142.90	530.0
144.80	236.0
148.00	117.0
171.90	530.0
172.80	471.0
173.90	30232.0
174.90	1907.0
175.90	28608.0
176.90	1702.0

Instrument :
MSVOA_U
ClientSampleId :
BFB063