

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU061518\
 Data File : VU024609.D
 Acq On : 15 Jun 2018 22:15
 Operator : MD/SY
 Sample : VU0615WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK45

Quant Time: Jun 16 03:44:37 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM061518WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 16 03:36:16 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	333045	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	297798	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.49	152	126093	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	92501	48.52	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	97.04%
7) Chloroethane-d5	1.68	69	74884	51.06	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	102.12%
11) 1,1-Dichloroethene-d2	2.28	63	133398	35.02	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	70.04%
21) 2-Butanone-d5	4.18	46	171880	106.82	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	106.82%
24) Chloroform-d	4.65	84	181741	47.32	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.64%
26) 1,2-Dichloroethane-d4	5.31	65	118660	49.26	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.52%
32) Benzene-d6	5.35	84	382218	52.71	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	105.42%
36) 1,2-Dichloropropane-d6	6.34	67	125678	52.25	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	104.50%
41) Toluene-d8	7.57	98	363281	49.65	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	99.30%
43) trans-1,3-Dichloropropene-	7.85	79	57159	46.57	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	93.14%
47) 2-Hexanone-d5	8.31	63	135182	109.16	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	109.16%
57) 1,1,2,2-Tetrachloroethane-	10.44	84	176206	49.94	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	99.88%
64) 1,2-Dichlorobenzene-d4	11.86	152	133613	54.92	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	109.84%


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
59) 1,2,3-Trichloropropane	11.49	75	14643	4.735	ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU061518\
Data File : VU024609.D
Acq On : 15 Jun 2018 22:15
Operator : MD/SY
Sample : VU0615WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK45

Quant Time: Jun 16 03:44:37 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM061518WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jun 16 03:36:16 2018
Response via : Initial Calibration

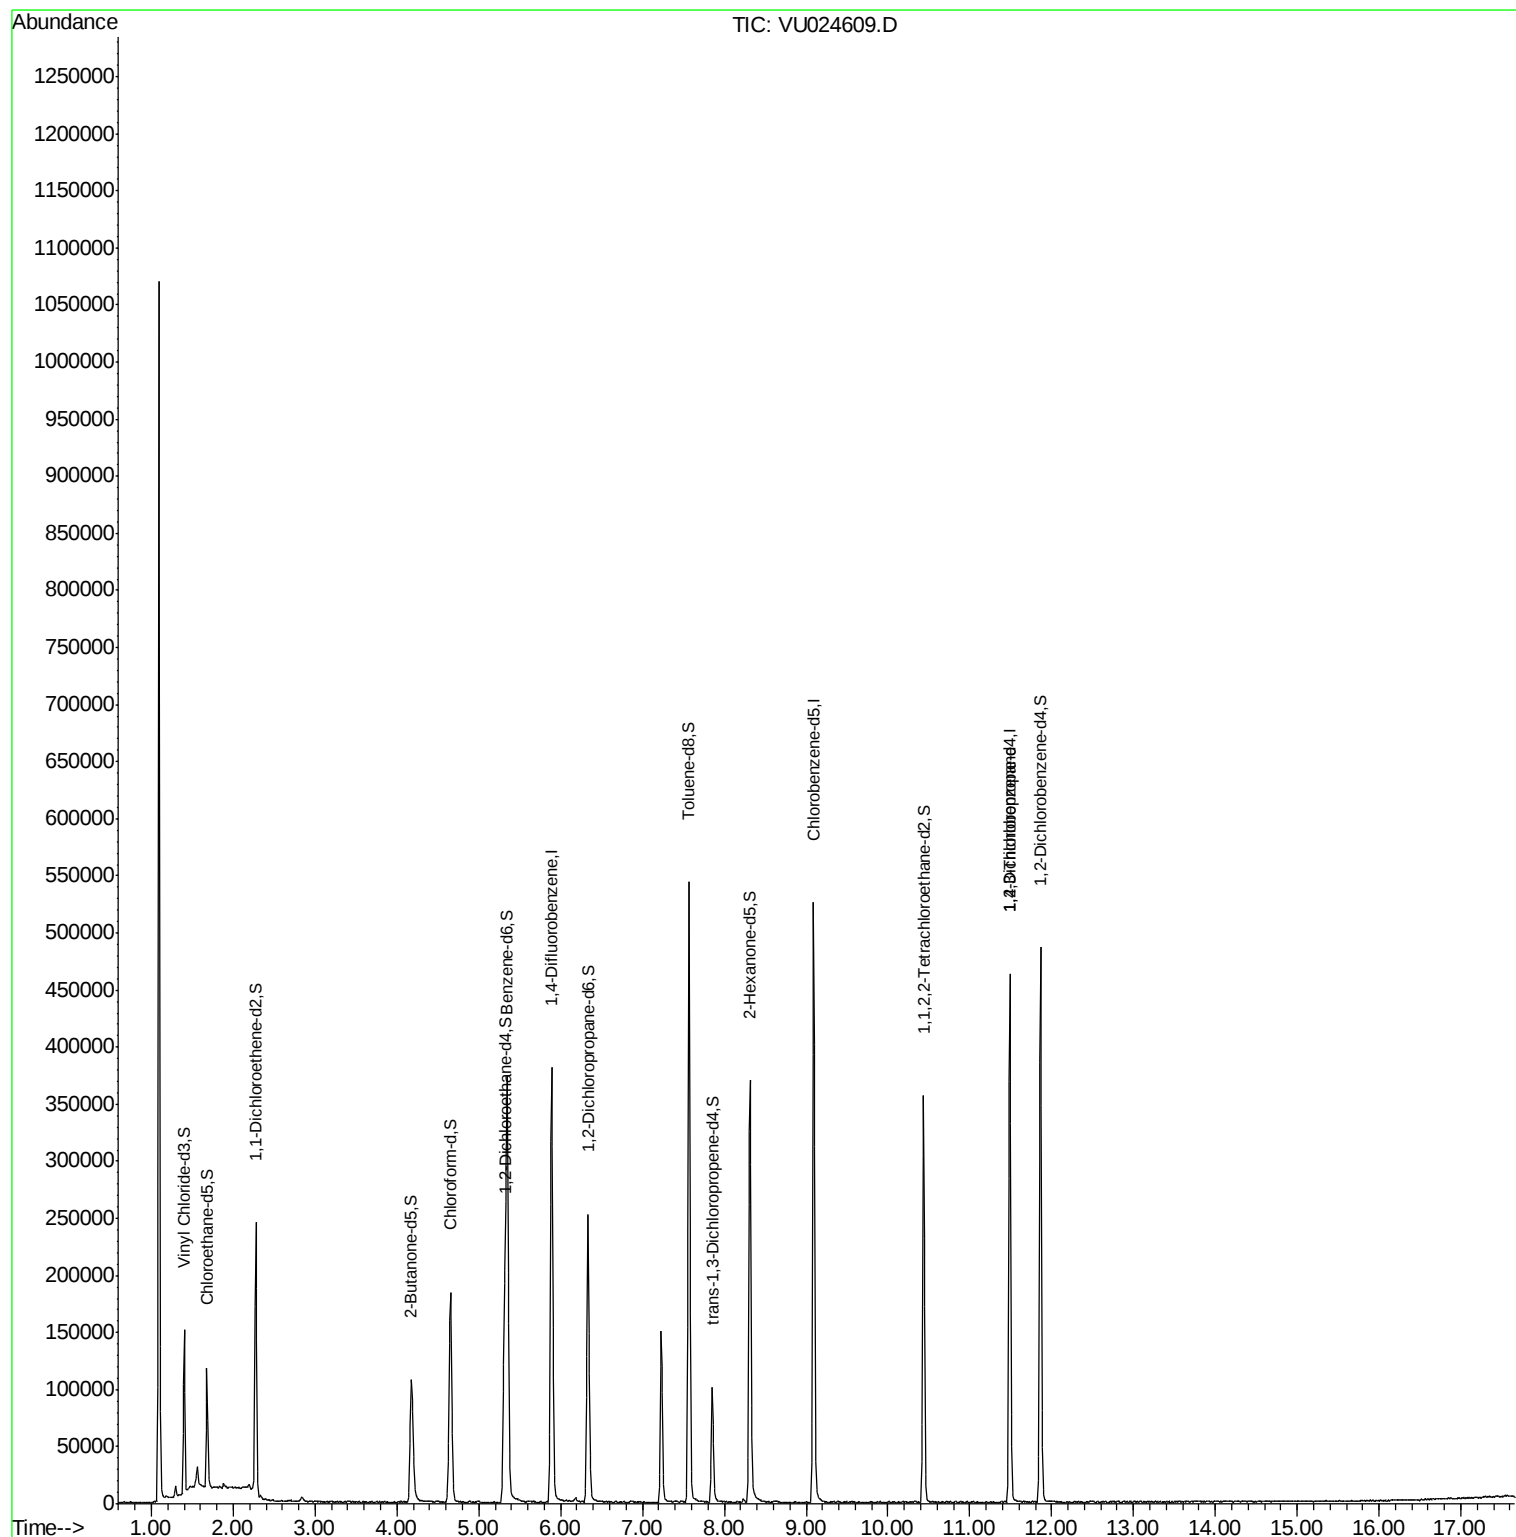

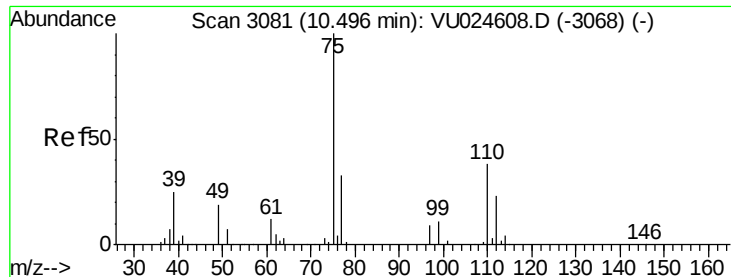

#59

1,2,3-Trichloropropane

Concen: 4.735 ug/L

RT: 11.49 min Scan# 3389

Delta R.T. 0.99 min

Lab File: VU024609.D

Acq: 15 Jun 2018 22:15

Instrument :

MSVOA_U

ClientSampleId :

VBLK45

Tgt Ion: 75 Resp: 14643

Ion Ratio Lower Upper

75 100

77 39.1 26.3 39.5

