

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061520\
 Data File : VU038900.D
 Acq On : 15 Jun 2020 18:42
 Operator : SY/MD
 Sample : L2975-03
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF8P7

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR061520WMA.M
 Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.613	77	85	93	rBV	96803	102915	1.30%	0.620%
2	1.748	118	127	138	rVB	135142	167713	2.12%	1.010%
3	1.932	175	184	196	rBV	97736	126696	1.60%	0.763%
4	2.591	377	389	405	rBV	176696	293374	3.70%	1.767%
5	4.677	1017	1038	1072	rBV	167538	554720	7.00%	3.342%
6	5.102	1154	1170	1193	rBV	187774	405180	5.11%	2.441%
7	5.758	1353	1374	1408	rBV2	343630	921947	11.63%	5.554%
8	6.279	1521	1536	1554	rBV	308946	598040	7.54%	3.603%
9	6.571	1608	1627	1660	rBV	4224756	7929031	100.00%	47.766%
10	6.719	1660	1673	1691	rVB2	222437	450603	5.68%	2.715%
11	7.591	1928	1944	1965	rBV	85336	149486	1.89%	0.901%
12	7.922	2032	2047	2074	rBV	381921	682859	8.61%	4.114%
13	8.201	2122	2134	2150	rBV	55404	95172	1.20%	0.573%
14	8.574	2237	2250	2262	rBV	152437	262625	3.31%	1.582%
15	8.658	2263	2276	2309	rVB2	687865	1334961	16.84%	8.042%
16	9.436	2505	2518	2536	rBV	467462	781523	9.86%	4.708%
17	10.770	2920	2933	2948	rVB	202778	325786	4.11%	1.963%
18	11.825	3248	3261	3281	rBV	454198	724867	9.14%	4.367%
19	12.204	3365	3379	3400	rBV	430609	692321	8.73%	4.171%




Sum of corrected areas: 16599819

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU061520\
Data File : VU038900.D
Acq On : 15 Jun 2020 18:42
Operator : SY/MD
Sample : L2975-03
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF8P7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR061520WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

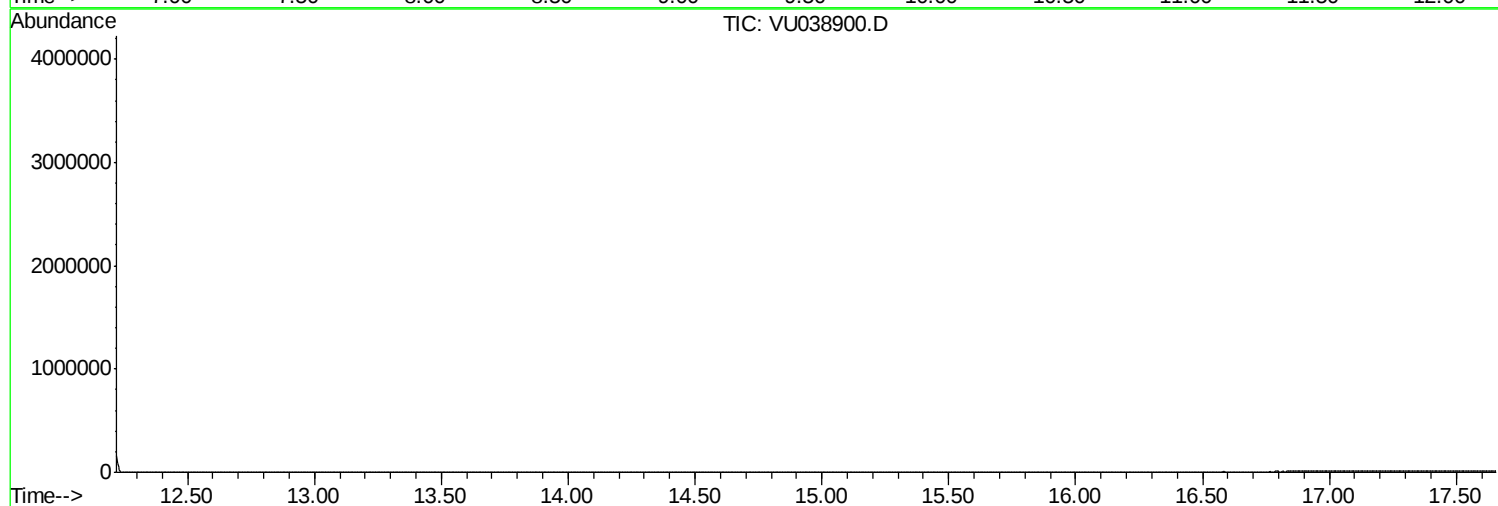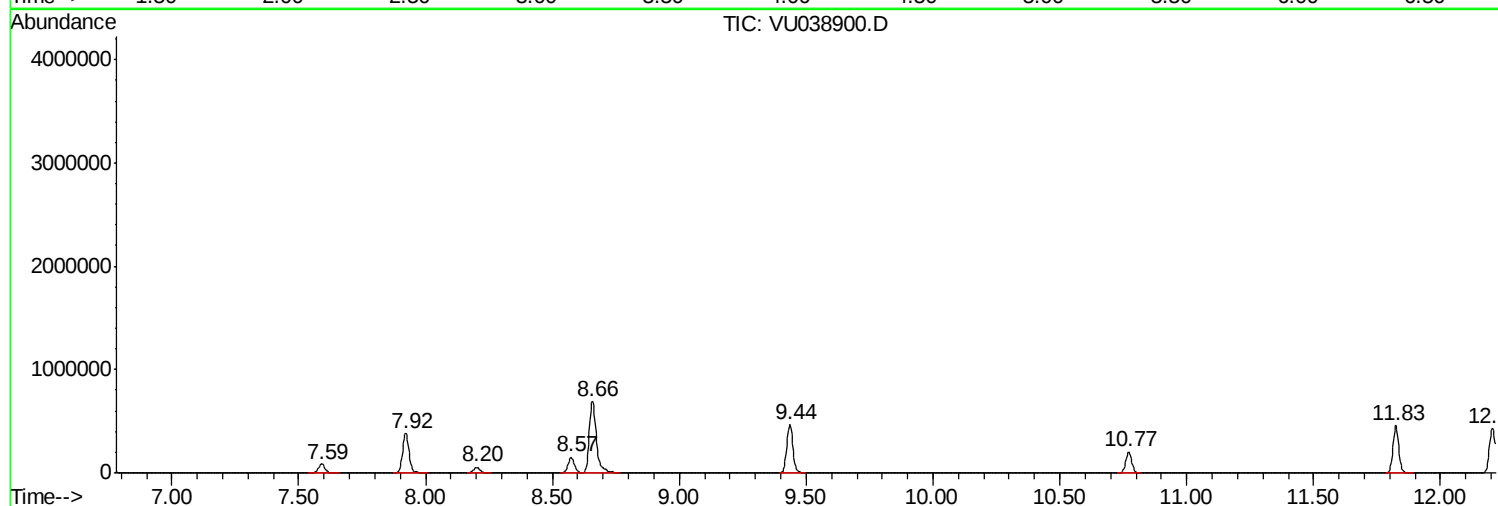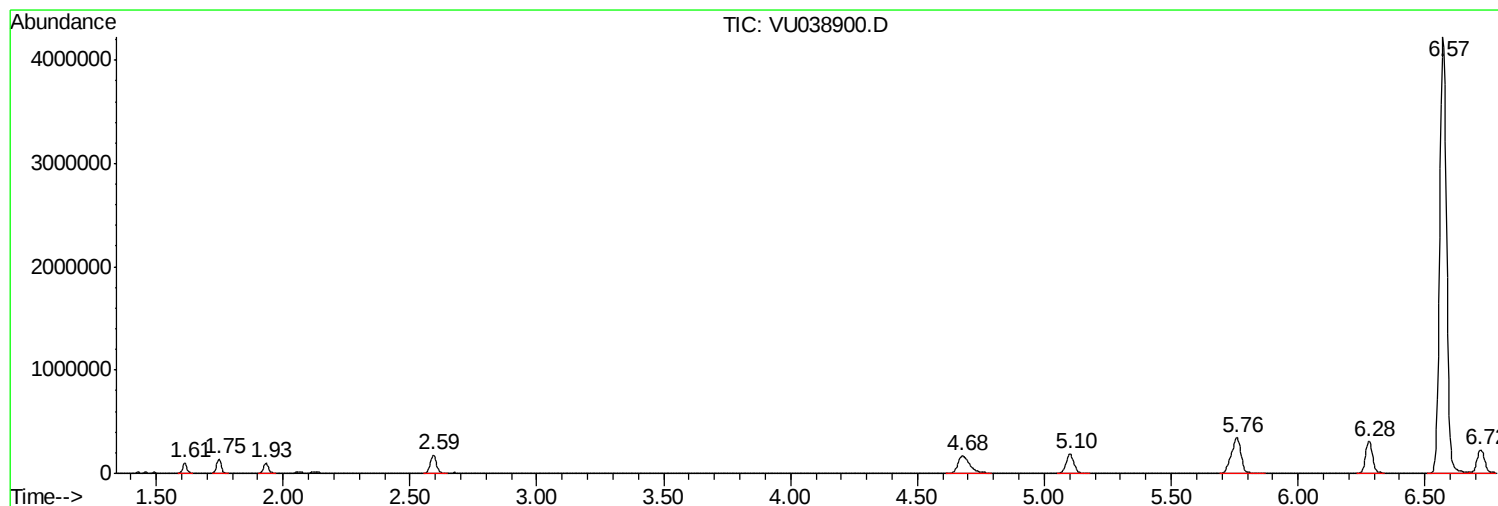

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061520\
Data File : VU038900.D
Acq On : 15 Jun 2020 18:42
Operator : SY/MD
Sample : L2975-03
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1










Instrument :
MSVOA_U
ClientSampleId :
BF8P7

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR061520WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Trimethylsilyl fluoride Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
1.75	1.40 ug/L	167713	1,4-Difluorobenzene	6.28	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Trimethylsilyl fluoride	92	C3H9FSi	000420-56-4	91
2	Trimethylsilyl fluoride	92	C3H9FSi	000420-56-4	90
3	Trimethylphosphine oxide	92	C3H9OP	000676-96-0	23
4	Propane, 1,2-dichloro-2-methyl-	126	C4H8Cl2	000594-37-6	9
5	Propane, 2-chloro-2-nitro-	123	C3H6ClNO2	000594-71-8	4

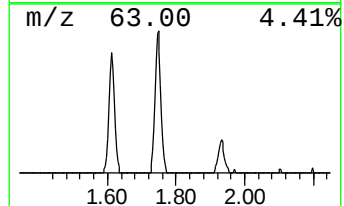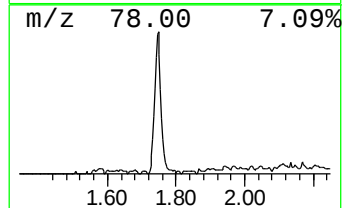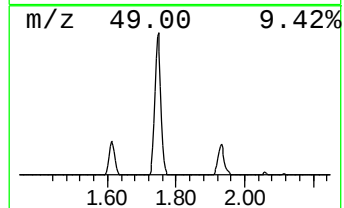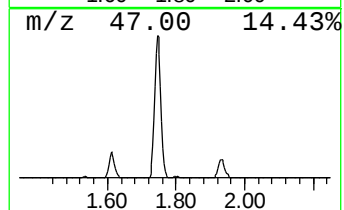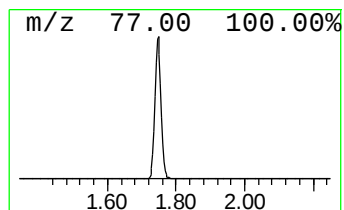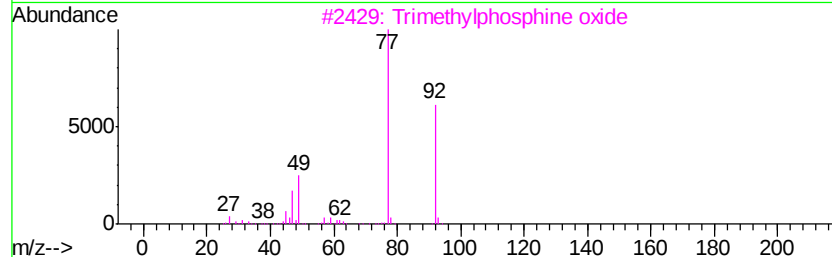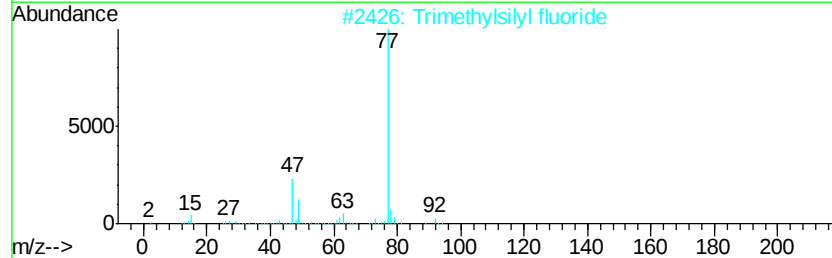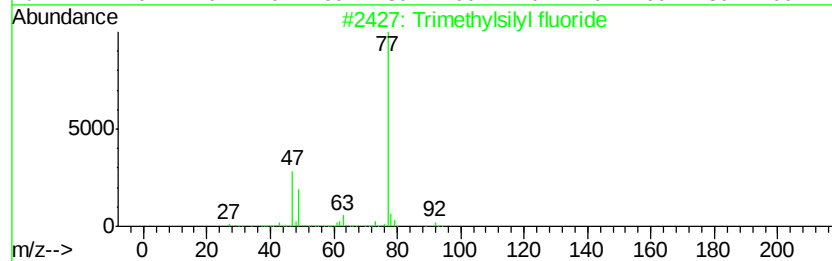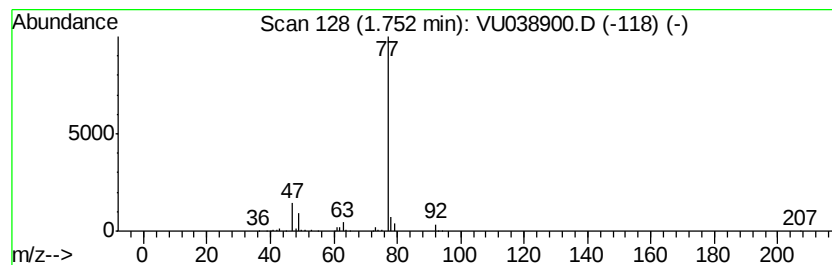

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU061520\
Data File : VU038900.D
Acq On : 15 Jun 2020 18:42
Operator : SY/MD
Sample : L2975-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF8P7

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR061520WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Trimethylsilyl fl...	1.75	1.4	ug/L	167713	1	6.28	598040	5.0