

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061520\
 Data File : VU038912.D
 Acq On : 15 Jun 2020 23:18
 Operator : SY/MD
 Sample : L2985-06DL 5X
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFT74DL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR061520WMA.M
 Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.610	76	84	98	rVB	124014	139486	9.83%	1.246%
2	1.932	176	184	198	rBV	132145	175215	12.35%	1.566%
3	2.153	245	253	262	rBV	43882	68606	4.83%	0.613%
4	2.584	374	387	403	rBV2	237189	397798	28.03%	3.555%
5	3.073	527	539	555	rVB2	16438	30916	2.18%	0.276%
6	3.218	567	584	602	rBV	35924	98222	6.92%	0.878%
7	4.694	1021	1043	1086	rBV3	167647	691448	48.72%	6.178%
8	5.099	1151	1169	1190	rBV	204391	448173	31.58%	4.005%
9	5.758	1352	1374	1408	rBV2	409383	1066449	75.15%	9.529%
10	6.279	1521	1536	1559	rBV	352437	677122	47.71%	6.050%
11	6.568	1612	1626	1645	rBV	367967	708323	49.91%	6.329%
12	6.719	1658	1673	1693	rBV	251358	489969	34.53%	4.378%
13	7.591	1930	1944	1962	rBV	121827	220340	15.53%	1.969%
14	7.922	2032	2047	2068	rBV	464958	821286	57.87%	7.339%
15	8.201	2121	2134	2151	rBV	85376	144376	10.17%	1.290%
16	8.571	2234	2249	2265	rBV	357585	631050	44.47%	5.639%
17	8.671	2265	2280	2308	rVB	597216	1419160	100.00%	12.681%
18	9.436	2505	2518	2545	rBV	548214	969460	68.31%	8.663%
19	10.774	2921	2934	2949	rBV	220119	359381	25.32%	3.211%
20	11.825	3249	3261	3278	rBV	512357	826699	58.25%	7.387%
21	12.204	3364	3379	3398	rBV	506744	807805	56.92%	7.218%


Sum of corrected areas: 11191284

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU061520\
Data File : VU038912.D
Acq On : 15 Jun 2020 23:18
Operator : SY/MD
Sample : L2985-06DL 5X
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFT74DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR061520WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

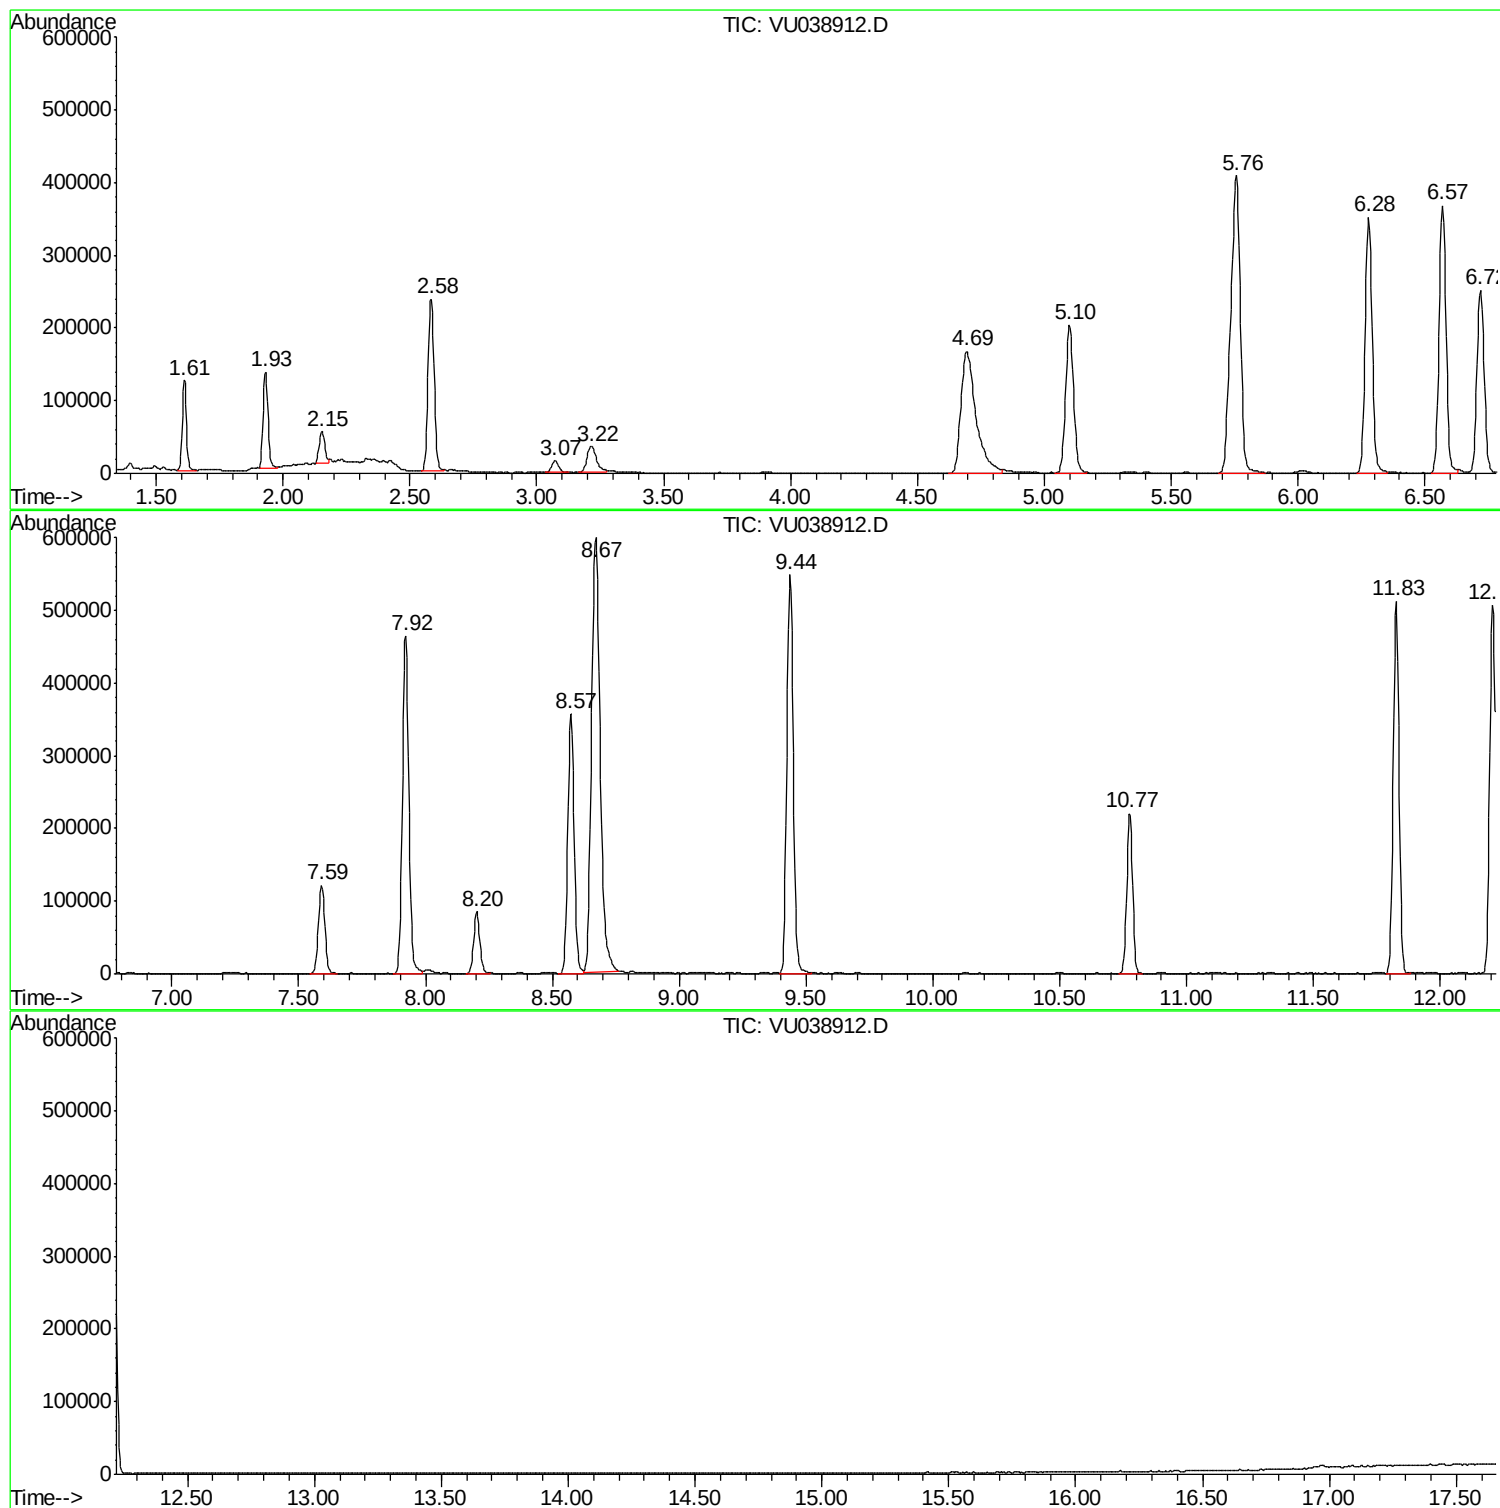

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU061520\
Data File : VU038912.D
Acq On : 15 Jun 2020 23:18
Operator : SY/MD
Sample : L2985-06DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFT74DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR061520WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_U\DATA\VU061520\
Data File : VU038912.D
Acq On : 15 Jun 2020 23:18
Operator : SY/MD
Sample : L2985-06DL 5X
Misc : 25.0mL/MSV0A_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_U
ClientSampleId :
BFT74DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_U\METHOD\SOMUTR061520WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc