

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061520\
 Data File : VU038913.D
 Acq On : 15 Jun 2020 23:41
 Operator : SY/MD
 Sample : L2985-08DL 10X
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFT76DL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR061520WMA.M
 Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.610	77	84	97	rVB	118226	132937	9.78%	1.256%
2	1.932	175	184	195	rBV	117904	158409	11.65%	1.497%
3	2.584	376	387	406	rBV	226457	365384	26.87%	3.453%
4	3.073	526	539	553	rBV2	14941	28746	2.11%	0.272%
5	3.218	568	584	602	rBV	33699	89936	6.61%	0.850%
6	4.697	1025	1044	1102	rBV3	169644	689262	50.69%	6.514%
7	5.102	1153	1170	1188	rBV	191471	428364	31.50%	4.049%
8	5.758	1352	1374	1412	rBV2	389492	1020012	75.01%	9.640%
9	6.279	1520	1536	1559	rBV	338228	649132	47.74%	6.135%
10	6.571	1611	1627	1655	rBV	421049	808258	59.44%	7.639%
11	6.719	1659	1673	1695	rVB	241823	471895	34.70%	4.460%
12	7.590	1929	1944	1961	rBV	120686	211773	15.57%	2.002%
13	7.922	2032	2047	2068	rBV	432971	766645	56.38%	7.246%
14	8.201	2122	2134	2152	rBV	78700	134179	9.87%	1.268%
15	8.571	2237	2249	2265	rBV	310662	541502	39.82%	5.118%
16	8.668	2265	2279	2312	rVB	589015	1359785	100.00%	12.852%
17	9.436	2502	2518	2539	rBV	493182	841156	61.86%	7.950%
18	10.774	2921	2934	2947	rBV	209538	345065	25.38%	3.261%
19	11.825	3244	3261	3278	rBV	496884	786951	57.87%	7.438%
20	12.204	3367	3379	3398	rVB	467053	751306	55.25%	7.101%


Sum of corrected areas: 10580697

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU061520\
Data File : VU038913.D
Acq On : 15 Jun 2020 23:41
Operator : SY/MD
Sample : L2985-08DL 10X
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFT76DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR061520WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

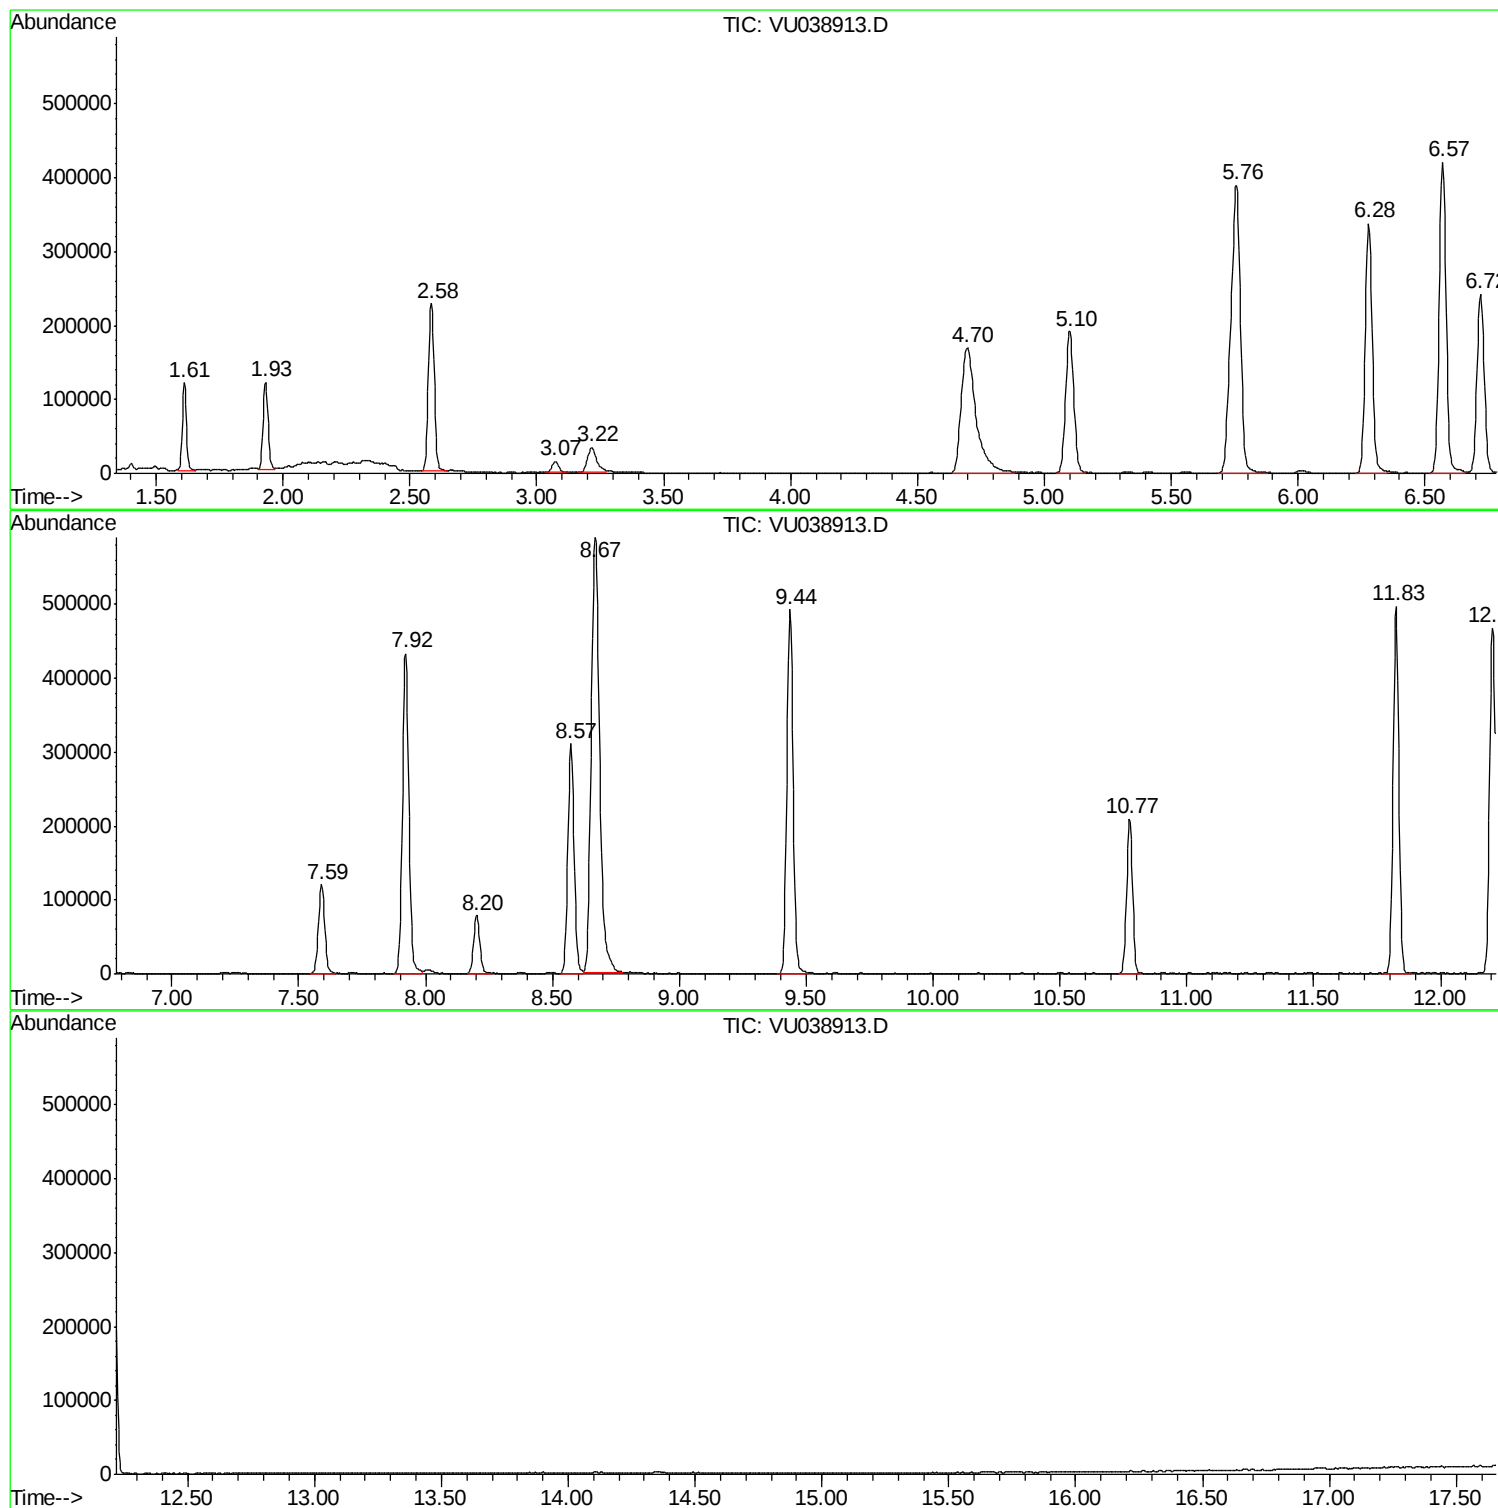

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU061520\
Data File : VU038913.D
Acq On : 15 Jun 2020 23:41
Operator : SY/MD
Sample : L2985-08DL 10X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFT76DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR061520WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU061520\
Data File : VU038913.D
Acq On : 15 Jun 2020 23:41
Operator : SY/MD
Sample : L2985-08DL 10X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFT76DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR061520WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc