


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061520\
 Data File : VU038883.D
 Acq On : 15 Jun 2020 08:56
 Operator : SY/MD
 Sample : BFB13
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB13

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR061520WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Jun 17 11:39:07 2020

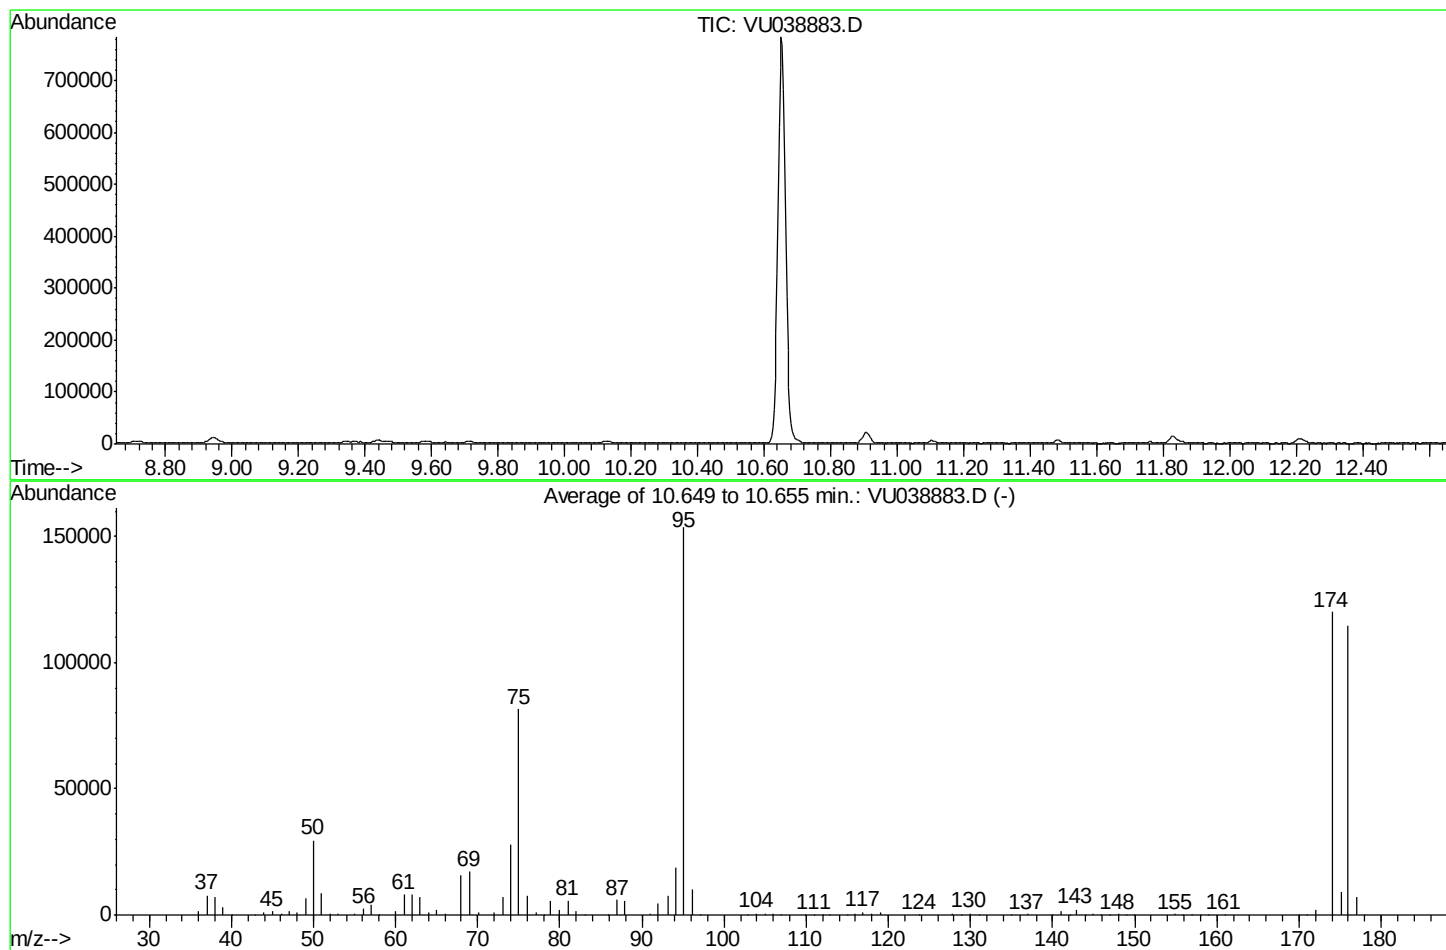

AutoFind: Scans 2895, 2896, 2897; Background Corrected with Scan 2881

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	29541	PASS
75	95	30	80	53.0	81482	PASS
95	95	100	100	100.0	153685	PASS
96	95	5	9	6.5	10016	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	78.2	120114	PASS
175	174	5	9	7.8	9353	PASS
176	174	95	101	95.4	114530	PASS
177	176	5	9	6.2	7088	PASS

m/z	Abundance
36.00	2249.0
37.00	7920.0
38.00	7160.0
39.00	2658.0
39.90	282.0
42.90	106.0
43.90	1433.0
45.00	1329.0
46.20	287.0
47.10	1469.0
48.00	943.0
49.00	6572.0
50.00	28416.0
51.00	8346.0
51.90	389.0
52.90	339.0
55.00	502.0
56.10	2374.0
57.00	3600.0
57.90	207.0
59.90	1568.0
61.00	7805.0
62.00	7537.0
63.00	6684.0
64.00	908.0
65.00	2165.0
66.00	282.0
68.00	14926.0
69.00	16656.0
70.00	1228.0
71.90	833.0
73.00	7283.0
74.00	26416.0
75.00	78736.0
76.00	7032.0
77.00	927.0
78.90	5267.0
79.90	1776.0
81.00	5311.0
81.90	1385.0
83.00	144.0
85.80	248.0
87.00	6143.0
87.90	5503.0
90.90	743.0
92.00	4582.0
93.10	7340.0
94.10	18312.0
95.10	145792.0
96.10	10129.0
97.00	222.0
104.00	693.0
105.00	246.0
105.90	665.0
106.90	134.0
109.90	128.0
111.00	175.0
112.00	131.0
112.70	164.0
115.00	163.0
115.90	661.0
116.90	1134.0
118.00	619.0
119.00	1098.0
123.80	198.0
127.80	515.0
128.90	297.0
129.90	536.0
131.10	207.0
134.90	288.0
137.00	370.0
139.90	155.0
141.00	1555.0
142.10	263.0
142.90	2089.0
144.00	182.0
145.00	662.0
145.90	136.0
148.00	327.0
149.00	113.0
149.90	147.0
154.90	334.0
155.90	109.0
157.00	296.0
158.90	131.0
160.90	168.0
170.90	203.0
172.10	2205.0
174.00	112496.0
175.10	8929.0
176.00	107328.0
177.00	6917.0

Instrument :
MSVOA_U
ClientSampleId :
BFB13

177.90

145.0

Instrument :
MSVOA_U
ClientSampleId :
BFB13

m/z	Abundance
36.00	2230.0
37.00	8196.0
38.00	7664.0
39.00	3036.0
39.90	284.0
42.90	155.0
43.90	1499.0
45.00	1317.0
46.00	329.0
47.00	1489.0
48.00	1025.0
49.00	7056.0
50.00	30640.0
51.00	9007.0
51.90	396.0
53.00	368.0
55.00	509.0
56.10	2582.0
57.00	3996.0
57.90	221.0
60.00	1746.0
61.00	8344.0
62.00	8147.0
63.00	7160.0
64.00	933.0
65.00	2235.0
66.00	304.0
68.00	16020.0
69.00	17536.0
70.10	1255.0
71.90	1013.0
73.00	7551.0
74.00	28672.0
75.00	84280.0
76.00	7725.0
77.10	869.0
78.90	5658.0
79.90	1908.0
81.00	5894.0
81.90	1603.0
83.00	142.0
85.90	221.0
87.00	6001.0
87.90	6087.0
91.00	689.0
92.00	4979.0
93.10	7819.0
94.10	19656.0
95.10	158976.0
96.10	10370.0
97.00	245.0
102.90	101.0
103.90	742.0
104.90	270.0
105.90	731.0
106.80	188.0
109.90	141.0
111.00	198.0
112.00	105.0
112.70	170.0
114.90	183.0
115.90	677.0
116.90	1215.0
118.00	648.0
119.00	1075.0
123.80	136.0
127.90	504.0
128.90	282.0
129.90	574.0
131.00	249.0
134.90	210.0
137.00	293.0
139.90	177.0
141.00	1509.0
142.00	282.0
142.90	2399.0
144.00	174.0
145.00	652.0
145.90	158.0
148.00	363.0
149.00	131.0
150.00	163.0
155.00	390.0
157.00	256.0
158.90	179.0
160.90	262.0
170.90	231.0
172.10	2302.0
174.00	123816.0
175.10	9737.0
176.00	118328.0
177.00	7236.0

Instrument :
MSVOA_U
ClientSampleId :
BFB13

178.00

175.0

Instrument :
MSVOA_U
ClientSampleId :
BFB13

m/z	Abundance
36.00	2022.0
37.00	7514.0
38.00	7299.0
39.00	3321.0
40.00	260.0
42.90	154.0
43.90	1392.0
45.00	1257.0
46.00	279.0
47.00	1568.0
48.10	1057.0
49.00	6668.0
50.00	29568.0
51.00	9056.0
52.00	345.0
53.00	329.0
55.00	454.0
56.10	2475.0
57.00	4070.0
57.90	210.0
60.00	1866.0
61.00	7977.0
62.00	8009.0
63.00	6860.0
64.00	934.0
65.00	1991.0
66.00	297.0
68.00	15725.0
69.00	16880.0
70.10	1141.0
72.00	1092.0
73.00	7238.0
74.00	27968.0
75.00	81432.0
76.00	7480.0
77.10	743.0
78.00	514.0
78.90	5643.0
80.00	1929.0
80.90	5875.0
81.90	1633.0
83.00	102.0
85.90	212.0
87.00	5637.0
87.90	5821.0
91.10	633.0
92.00	4883.0
93.10	7382.0
94.10	18768.0
95.10	156288.0
96.10	9549.0
97.00	238.0
103.90	725.0
105.00	304.0
105.90	697.0
106.80	197.0
109.90	115.0
110.90	193.0
112.10	107.0
112.80	156.0
114.90	217.0
115.90	622.0
116.90	1211.0
118.00	642.0
119.00	902.0
127.90	573.0
128.90	226.0
129.90	582.0
131.00	223.0
134.90	230.0
136.90	233.0
139.90	163.0
141.00	1456.0
142.00	255.0
142.90	2275.0
144.00	173.0
145.00	498.0
145.90	210.0
146.90	113.0
148.00	427.0
149.00	103.0
150.00	178.0
155.00	426.0
156.90	203.0
158.00	109.0
158.90	190.0
161.00	304.0
170.00	111.0
170.90	207.0
172.00	2361.0
174.00	124032.0
175.10	9395.0

Instrument :
MSVOA_U
ClientSampleId :
BFB13

176.00117936.0

177.007112.0

177.90227.0

Instrument :
MSVOA_U
ClientSampleId :
BFB13

Scan 2881 (10.604 min): VU038883.D
BFB13

m/z	Abundance
36.00	649.0
37.90	295.0
40.00	180.0
43.80	419.0

Instrument :
MSVOA_U
ClientSampleId :
BFB13