
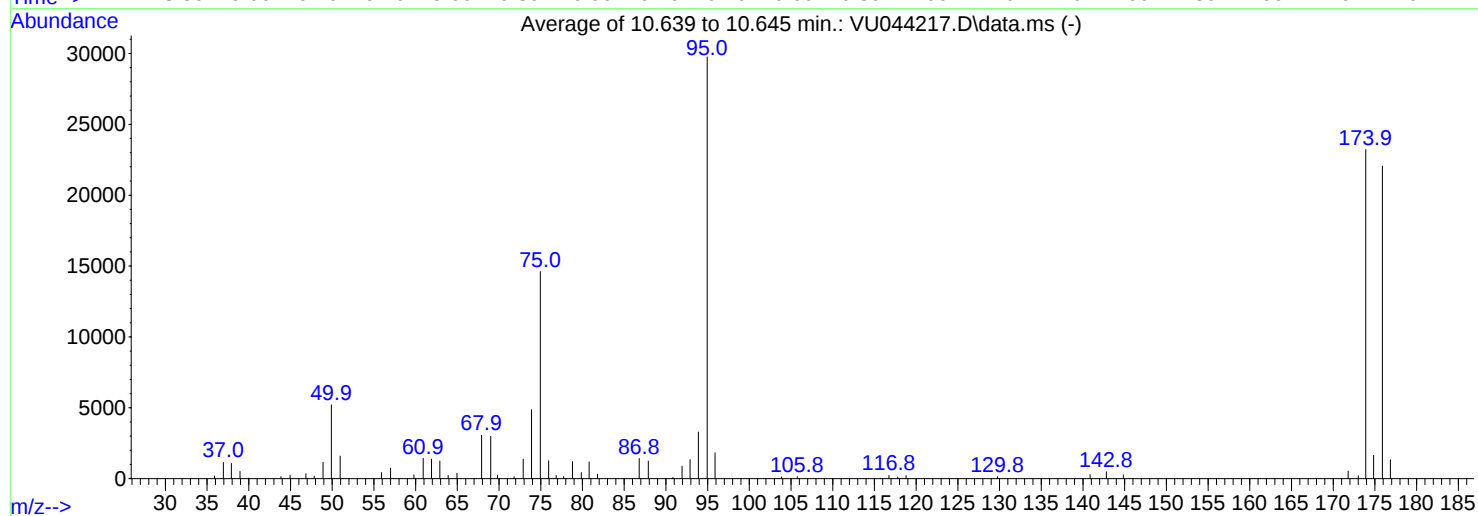


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061521\
Data File : VU044217.D
Acq On : 15 Jun 2021 10:25
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U060921W.M
Title : SW846 8260
Last Update : Thu Jun 10 05:11:37 2021

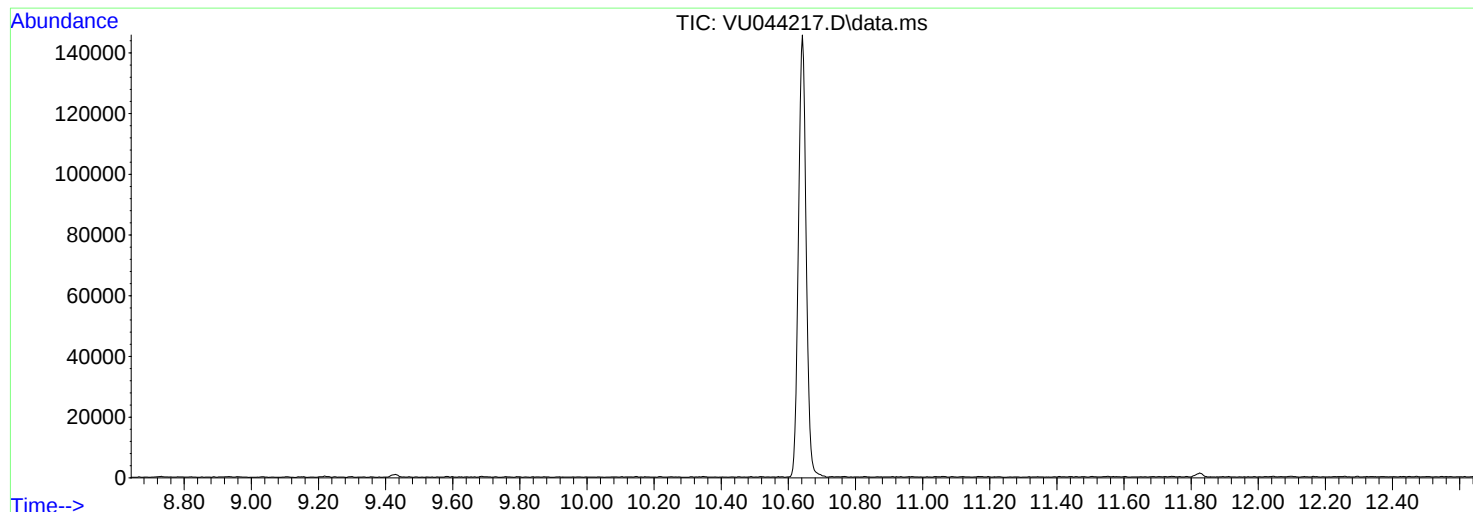

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2879

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.5	5205	PASS
75	95	30	60	49.1	14613	PASS
95	95	100	100	100.0	29763	PASS
96	95	5	9	6.1	1830	PASS
173	174	0.00	2	0.9	198	PASS
174	95	50	100	78.0	23221	PASS
175	174	5	9	7.1	1654	PASS
176	174	95	101	95.0	22061	PASS
177	176	5	9	6.1	1338	PASS