

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061523\
 Data File : VU054552.D
 Acq On : 16 Jun 2023 02:46
 Operator : MD/SY
 Sample : 03232-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 CONL1

Quant Time: Jun 16 04:25:44 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 14 00:05:43 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	251780	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.415	117	244817	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	119236	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.599	65	54295	3.388	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	67.800%
7) Chloroethane-d5	1.914	69	72918	4.860	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.200%
11) 1,1-Dichloroethene-d2	2.567	65	27423	3.832	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	76.600%
20) 2-Butanone-d5	4.631	46	226154	50.199	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	100.400%
24) Chloroform-d	5.058	84	161236	4.814	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.200%
26) 1,2-Dichloroethane-d4	5.698	65	85172	5.217	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.400%
32) Benzene-d6	5.724	84	314650	4.623	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.400%
36) 1,2-Dichloropropane-d6	6.689	67	109096	4.800	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.000%
41) Toluene-d8	7.894	98	254698	4.217	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.400%
43) trans-1,3-Dichloroprop...	8.177	79	30076	3.805	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	76.200%
46) 2-Hexanone-d5	8.631	63	148752	44.862	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	89.720%
56) 1,1,2,2-Tetrachloroeth...	10.753	84	82312	4.857	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.200%
66) 1,2-Dichlorobenzene-d4	12.190	152	99195	4.932	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.600%
Target Compounds						Qvalue
29) 1,1,1-Trichloroethane	5.312	97	5645	0.170	ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061523\
Data File : VU054552.D
Acq On : 16 Jun 2023 02:46
Operator : MD/SY
Sample : 03232-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
CONL1

Quant Time: Jun 16 04:25:44 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 14 00:05:43 2023
Response via : Initial Calibration

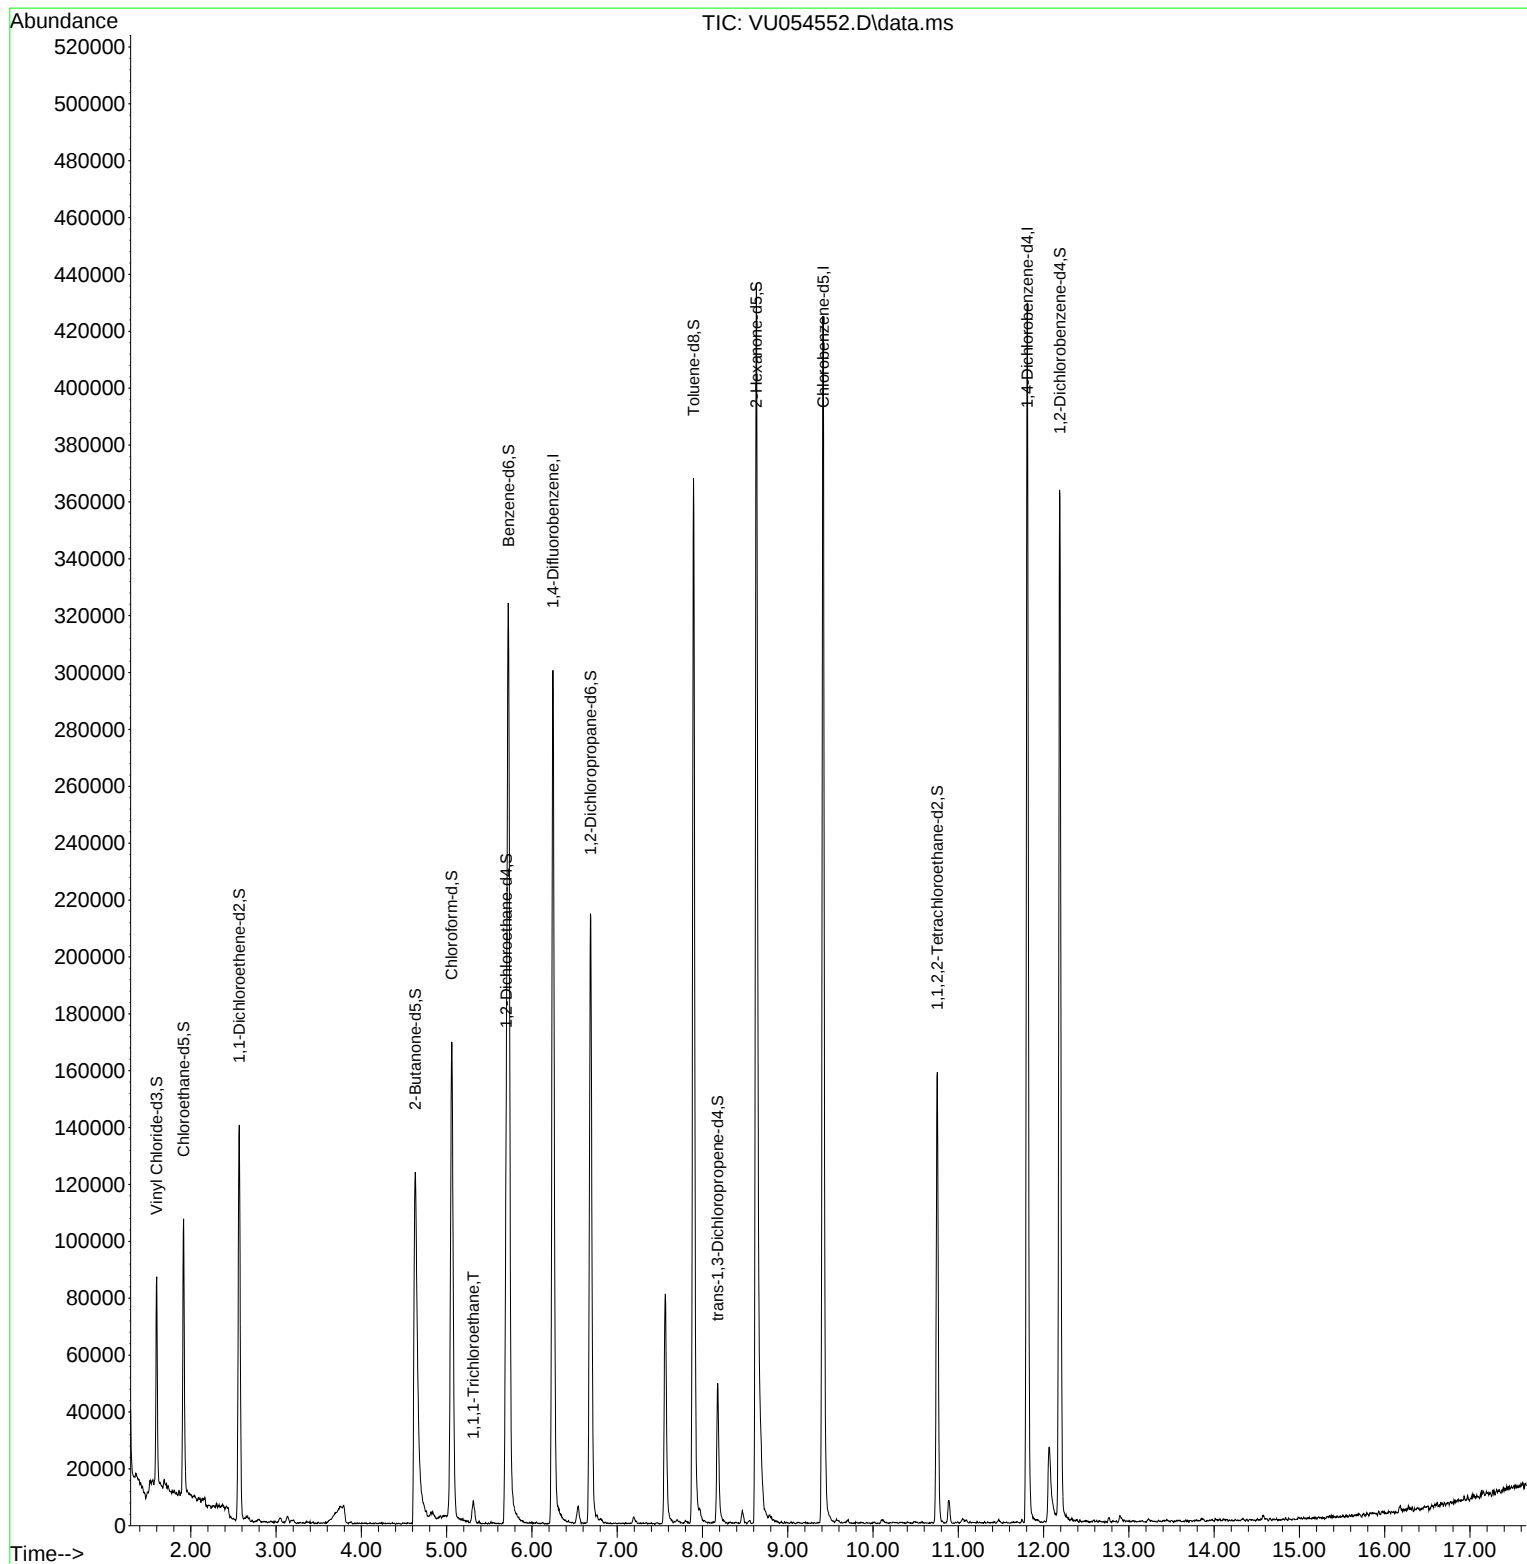

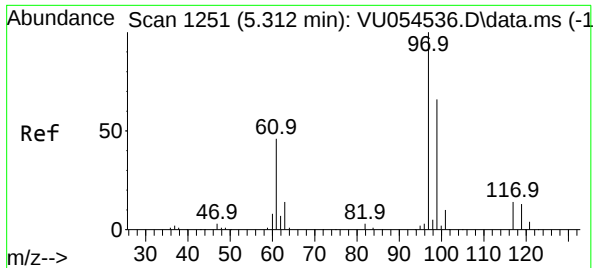

#29
 1,1,1-Trichloroethane
 Concen: 0.170 ug/L
 RT: 5.312 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: VU054552.D
 Acq: 16 Jun 2023 02:46

Instrument :
 MSVOA_U
 ClientSampleId :
 CONL1

Tgt Ion: 97	Resp:	5645
Ion	Ratio	Lower Upper
97	100	
99	69.5	50.8 76.2
61	53.0	36.1 54.1

