

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061523\
 Data File : VU054514.D
 Acq On : 15 Jun 2023 10:14
 Operator : MD/SY
 Sample : VU0615WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK002

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU054514.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	88	95	107	rBV	102448	120743	11.75%	1.480%
2	1.911	185	193	209	rBV	120321	162859	15.84%	1.996%
3	2.563	384	396	410	rBV	180892	297425	28.94%	3.644%
4	3.039	535	544	556	rBV2	8441	15713	1.53%	0.193%
5	4.624	1025	1037	1073	rBV	143135	414136	40.29%	5.075%
6	5.058	1156	1172	1193	rBV2	194310	443461	43.15%	5.434%
7	5.721	1358	1378	1408	rBV2	389228	1027834	100.00%	12.595%
8	6.245	1525	1541	1559	rBV	329667	635202	61.80%	7.783%
9	6.534	1620	1631	1643	rVB	5158	10446	1.02%	0.128%
10	6.685	1664	1678	1695	rBV	256551	505021	49.13%	6.188%
11	7.563	1939	1951	1974	rBV2	100171	185078	18.01%	2.268%
12	7.894	2040	2054	2073	rBV	440645	777837	75.68%	9.531%
13	8.177	2130	2142	2162	rBV	59140	109505	10.65%	1.342%
14	8.630	2267	2283	2319	rBV2	475525	967860	94.17%	11.860%
15	9.415	2513	2527	2550	rBV	443575	776660	75.56%	9.517%
16	10.753	2931	2943	2958	rBV	176803	287750	28.00%	3.526%
17	11.807	3259	3271	3294	rVV	438683	722131	70.26%	8.849%
18	12.190	3373	3390	3407	rBV	393308	659074	64.12%	8.076%
19	13.843	3896	3904	3915	rBV5	8867	14146	1.38%	0.173%
20	14.097	3970	3983	3994	rBV3	6052	11890	1.16%	0.146%
21	14.331	4045	4056	4069	rBV7	8834	16178	1.57%	0.198%




Sum of corrected areas: 8160949

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061523\
Data File : VU054514.D
Acq On : 15 Jun 2023 10:14
Operator : MD/SY
Sample : VU0615WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

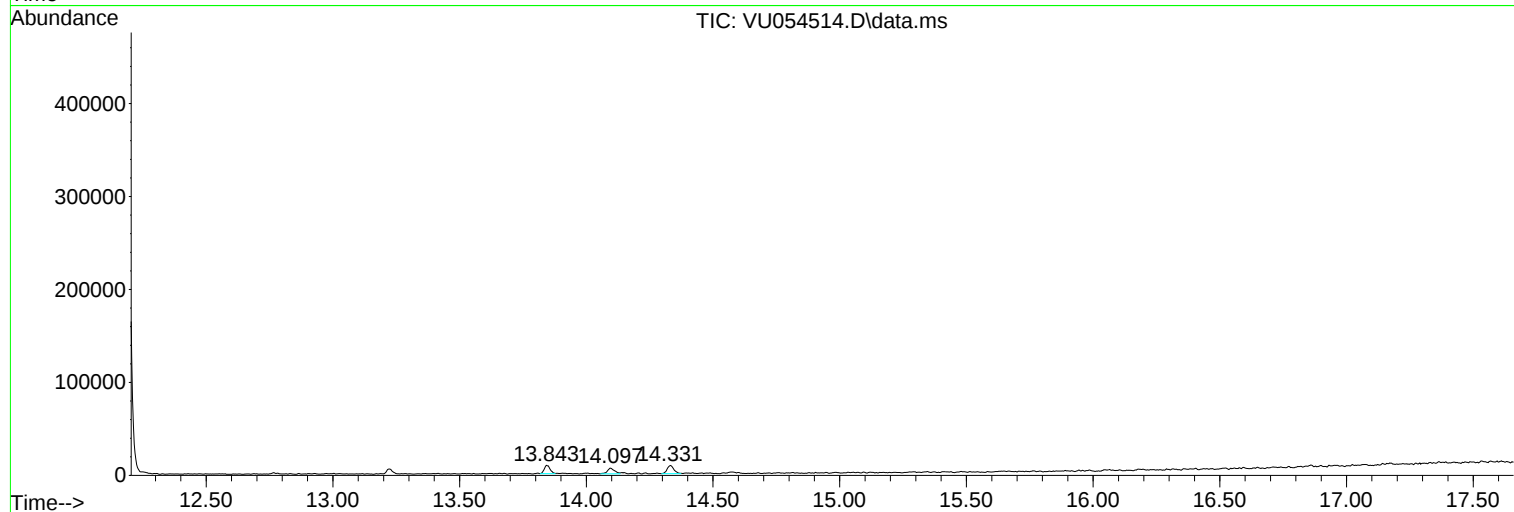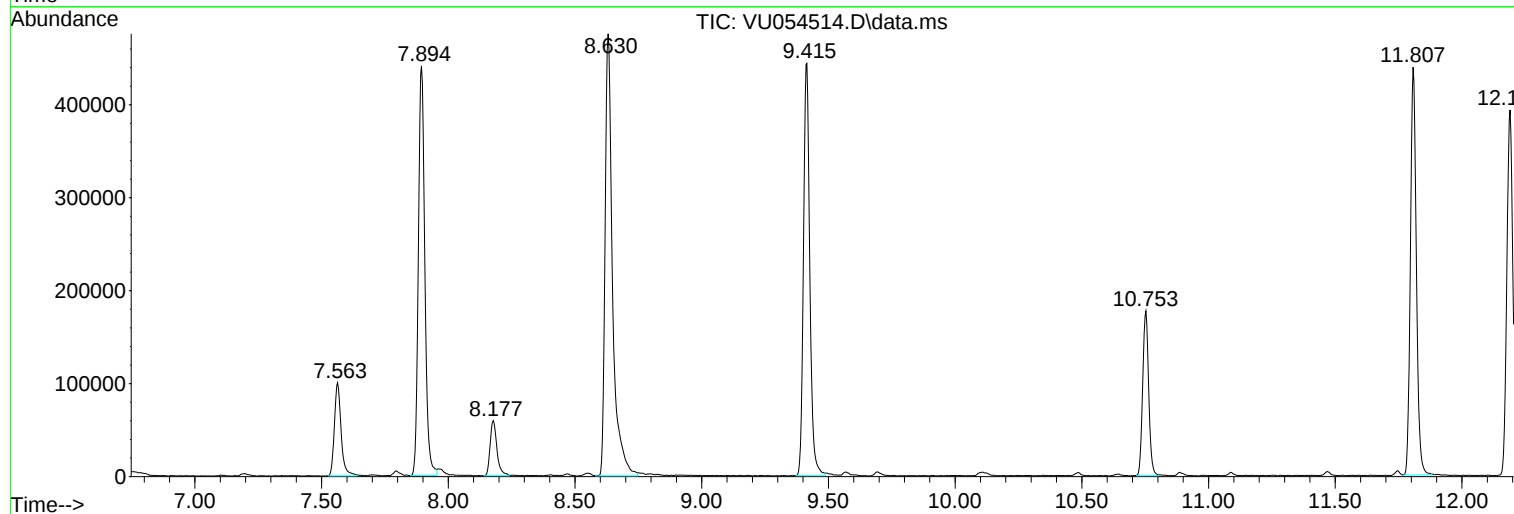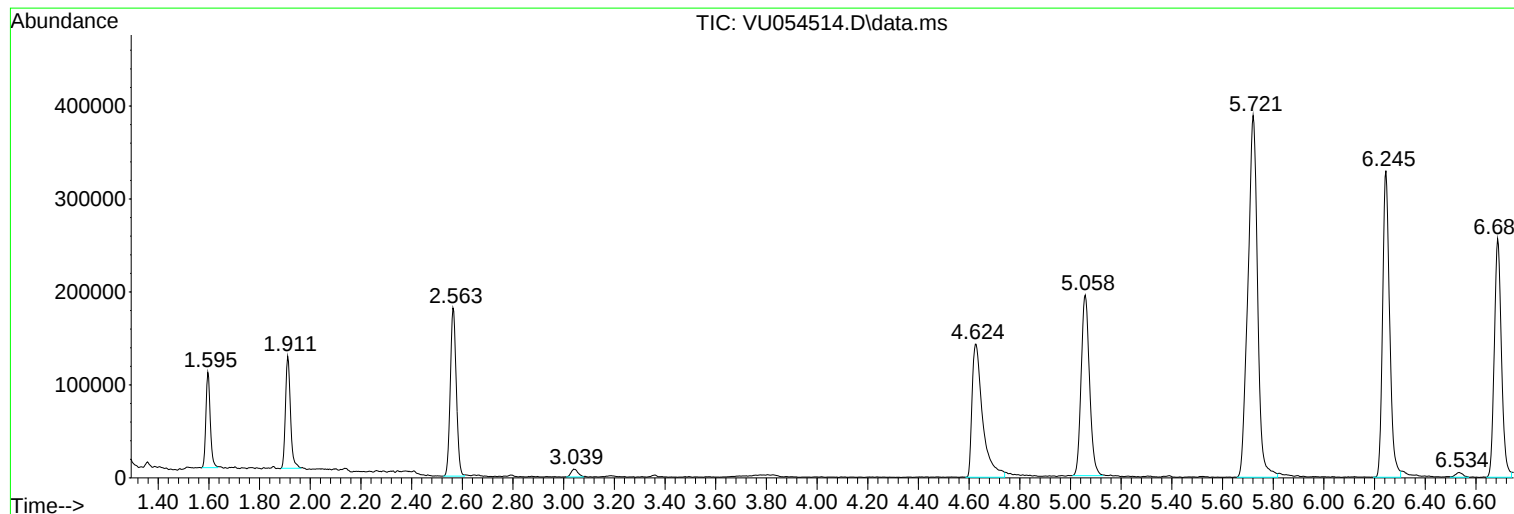

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061523\
Data File : VU054514.D
Acq On : 15 Jun 2023 10:14
Operator : MD/SY
Sample : VU0615WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061523\
Data File : VU054514.D
Acq On : 15 Jun 2023 10:14
Operator : MD/SY
Sample : VU0615WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc