

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061523\
 Data File : VU054525.D
 Acq On : 15 Jun 2023 14:46
 Operator : MD/SY
 Sample : 03253-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXYX0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU054525.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	89	96	108	rVB	68273	82227	4.47%	0.840%
2	1.914	186	194	206	rBV	75136	100232	5.45%	1.024%
3	2.567	385	397	414	rBV2	139567	247132	13.44%	2.524%
4	3.354	631	642	659	rBV5	15352	34534	1.88%	0.353%
5	3.866	786	801	822	rBV2	118849	283038	15.40%	2.890%
6	4.628	1025	1038	1074	rBV3	155029	575438	31.30%	5.876%
7	5.059	1156	1172	1196	rBV	159626	363696	19.79%	3.714%
8	5.313	1231	1251	1272	rBV	808523	1838167	100.00%	18.771%
9	5.724	1358	1379	1399	rBV2	291881	782421	42.57%	7.990%
10	6.245	1526	1541	1569	rBV	336102	671117	36.51%	6.853%
11	6.541	1621	1633	1649	rBV2	47744	91220	4.96%	0.932%
12	6.685	1664	1678	1704	rBV	205457	407849	22.19%	4.165%
13	7.563	1939	1951	1966	rBV2	87379	162523	8.84%	1.660%
14	7.894	2041	2054	2073	rBV	331518	591210	32.16%	6.037%
15	8.181	2131	2143	2160	rBV2	53389	97625	5.31%	0.997%
16	8.631	2272	2283	2318	rBV2	479200	977722	53.19%	9.984%
17	9.415	2513	2527	2552	rBV	473139	826176	44.95%	8.437%
18	10.753	2931	2943	2960	rBV2	169440	276852	15.06%	2.827%
19	11.807	3259	3271	3296	rBV	482939	792870	43.13%	8.097%
20	12.190	3377	3390	3413	rBV	355974	590646	32.13%	6.031%




Sum of corrected areas: 9792695

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061523\
Data File : VU054525.D
Acq On : 15 Jun 2023 14:46
Operator : MD/SY
Sample : 03253-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXYX0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

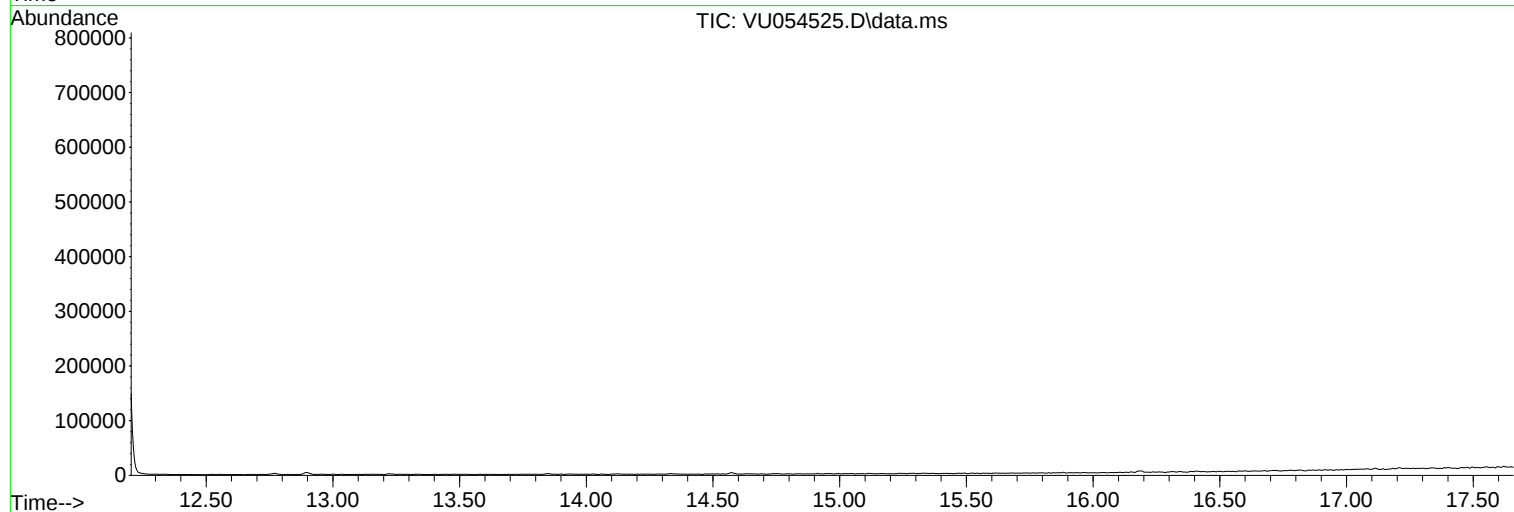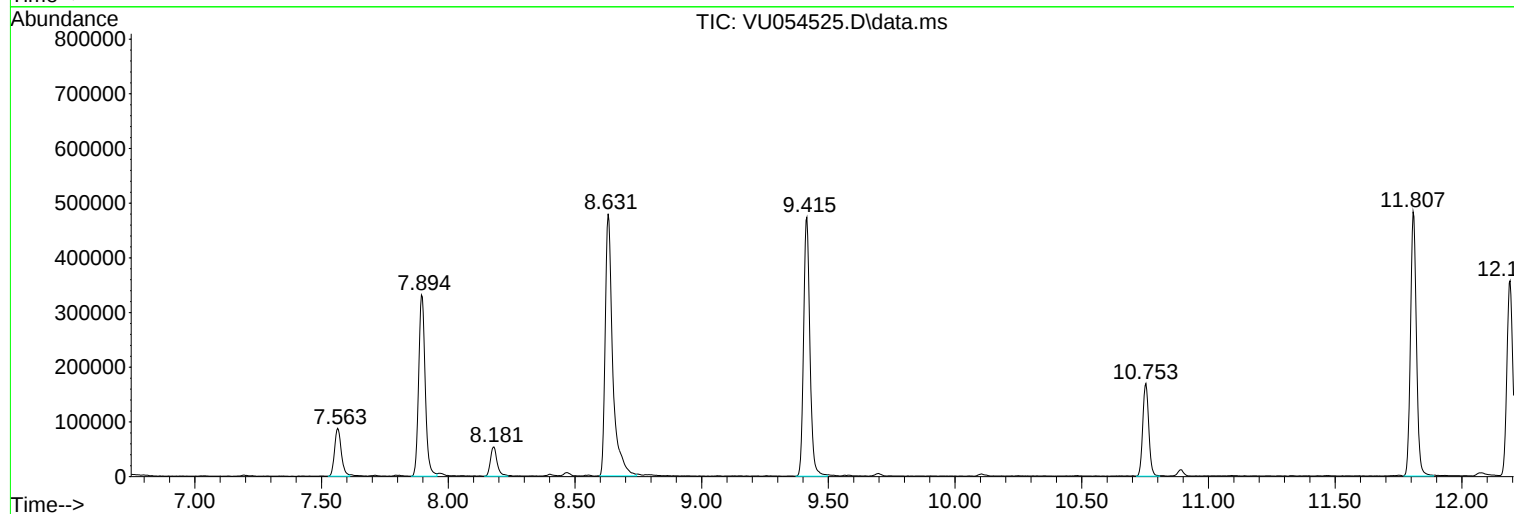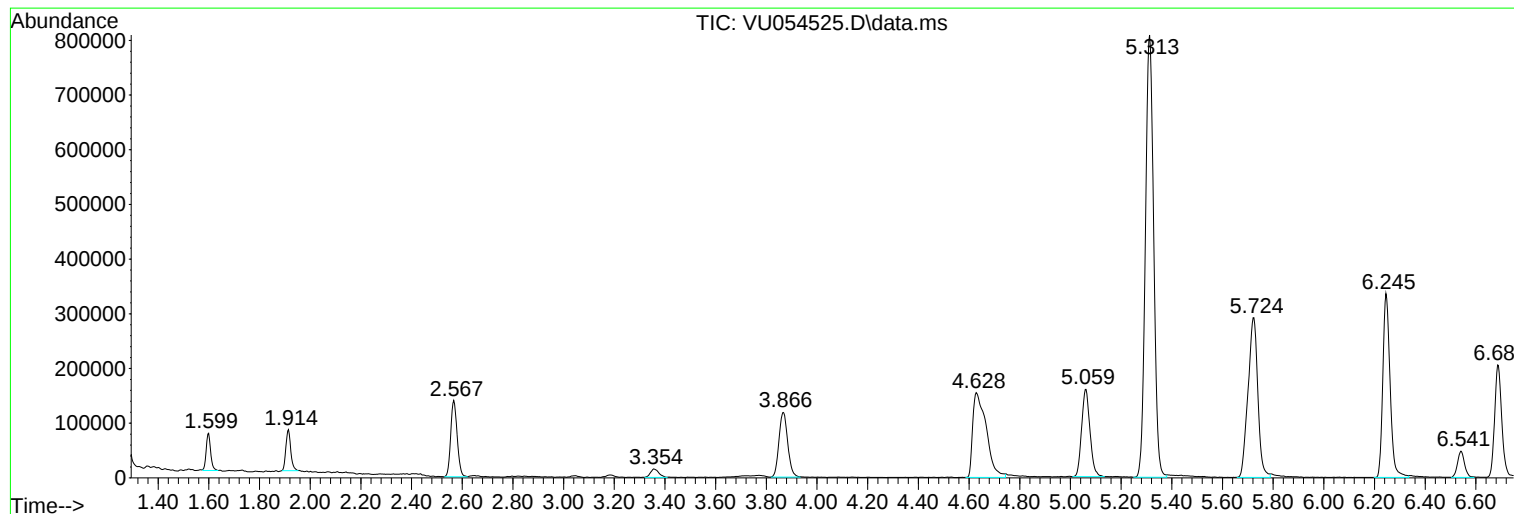

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061523\
Data File : VU054525.D
Acq On : 15 Jun 2023 14:46
Operator : MD/SY
Sample : 03253-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXYX0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061523\
Data File : VU054525.D
Acq On : 15 Jun 2023 14:46
Operator : MD/SY
Sample : 03253-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXYX0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------