

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061523\
 Data File : VU054537.D
 Acq On : 15 Jun 2023 20:32
 Operator : MD/SY
 Sample : VU0615WBL02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK003

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU054537.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	88	96	110	rVB	89463	106586	11.45%	1.379%
2	1.914	186	194	216	rVB	107216	148021	15.90%	1.914%
3	2.566	384	397	413	rBV	166101	276334	29.68%	3.574%
4	3.046	536	546	562	rVB4	6742	13124	1.41%	0.170%
5	3.181	574	588	604	rBV	5820	12668	1.36%	0.164%
6	4.631	1025	1039	1082	rBV	139817	427711	45.94%	5.532%
7	5.058	1156	1172	1196	rVB	180724	410061	44.04%	5.303%
8	5.721	1355	1378	1406	rBV2	355476	931118	100.00%	12.043%
9	6.245	1522	1541	1561	rBV	334575	652502	70.08%	8.439%
10	6.688	1664	1679	1697	rBV	228572	461190	49.53%	5.965%
11	7.563	1938	1951	1971	rBV	92088	170655	18.33%	2.207%
12	7.894	2040	2054	2074	rBV	396349	705351	75.75%	9.123%
13	8.177	2128	2142	2157	rBV	53103	98634	10.59%	1.276%
14	8.631	2271	2283	2318	rBV2	445133	908589	97.58%	11.751%
15	9.415	2511	2527	2552	rBV	454401	790610	84.91%	10.225%
16	10.753	2930	2943	2961	rBV	164562	270508	29.05%	3.499%
17	11.807	3260	3271	3293	rBV	435965	715888	76.88%	9.259%
18	12.190	3377	3390	3414	rBV2	350420	594627	63.86%	7.691%
19	13.843	3896	3904	3914	rBV6	8359	13440	1.44%	0.174%
20	14.097	3975	3983	3995	rBV3	5588	10161	1.09%	0.131%
21	14.328	4047	4055	4067	rBV5	8416	14136	1.52%	0.183%




Sum of corrected areas: 7731914

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061523\
Data File : VU054537.D
Acq On : 15 Jun 2023 20:32
Operator : MD/SY
Sample : VU0615WBL02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK003

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

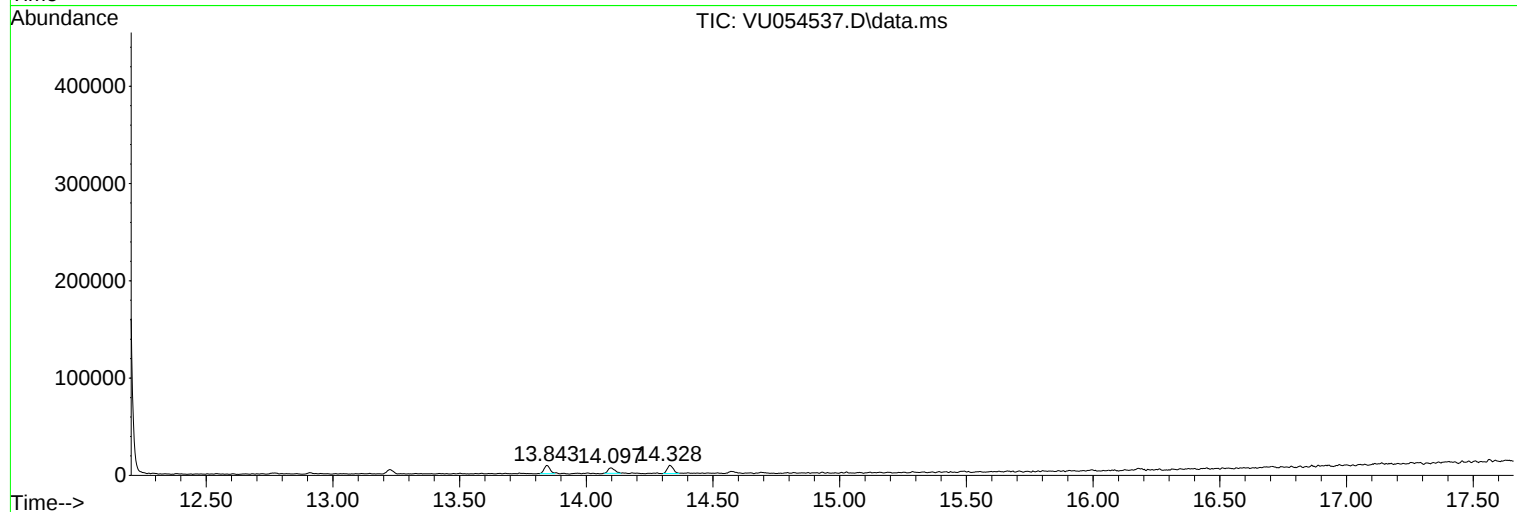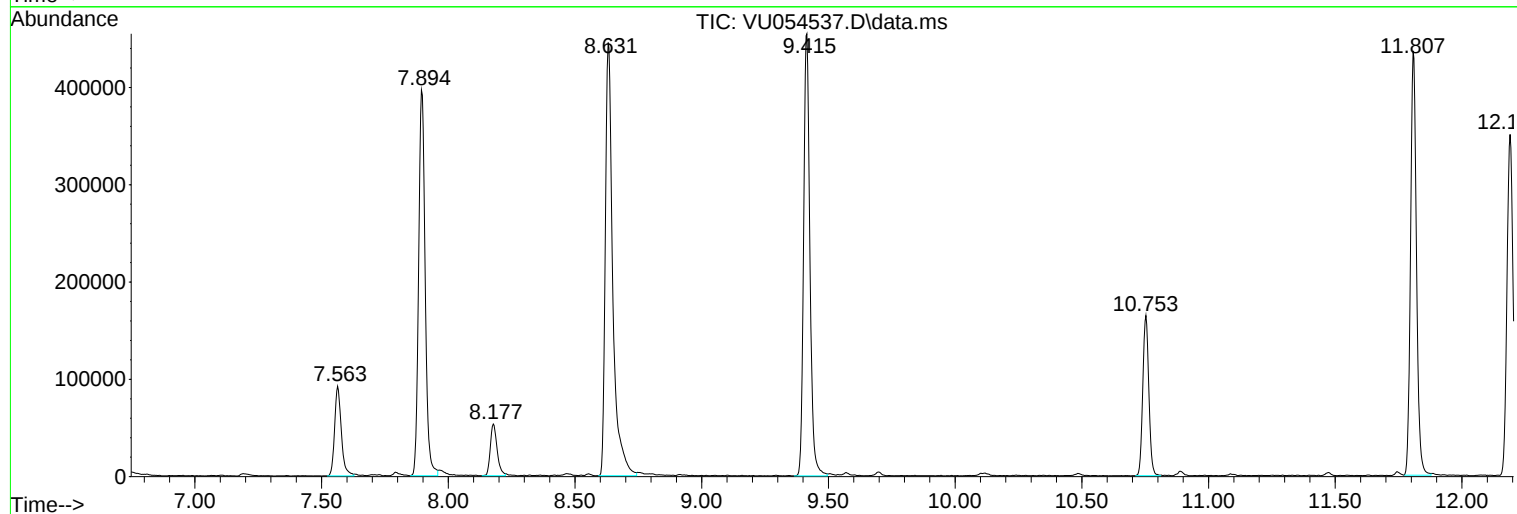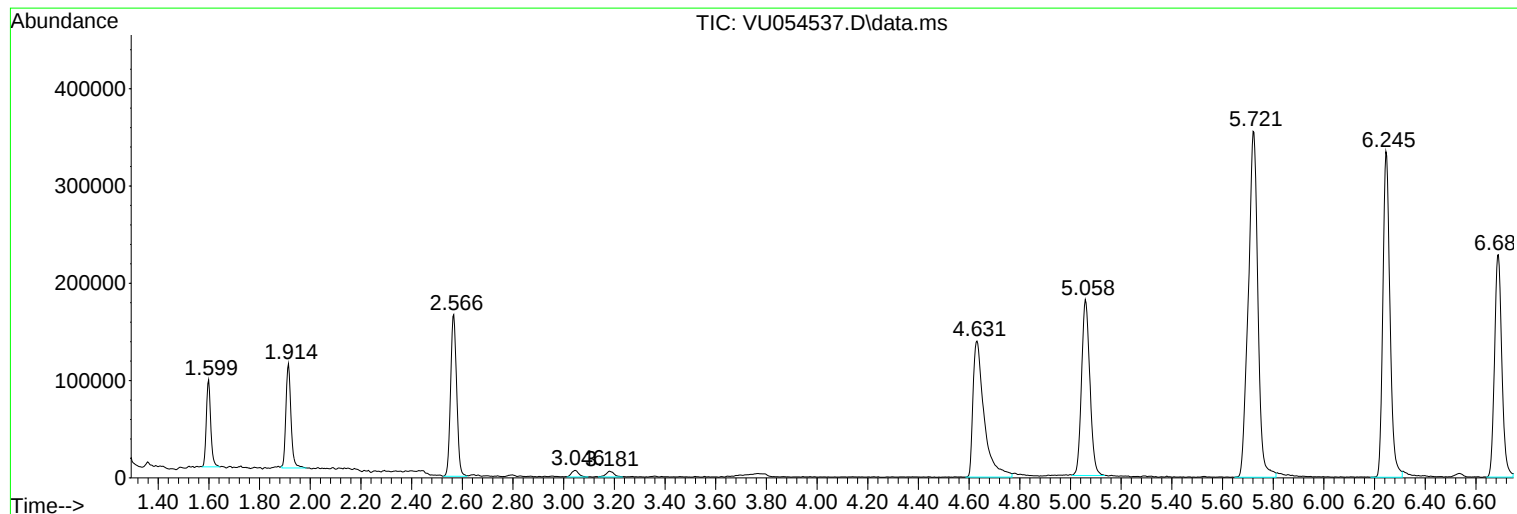

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061523\
Data File : VU054537.D
Acq On : 15 Jun 2023 20:32
Operator : MD/SY
Sample : VU0615WBL02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK003

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061523\
Data File : VU054537.D
Acq On : 15 Jun 2023 20:32
Operator : MD/SY
Sample : VU0615WBL02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK003

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------