

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061523\
 Data File : VU054538.D
 Acq On : 15 Jun 2023 21:06
 Operator : MD/SY
 Sample : 03253-13
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXYW6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU054538.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.380	23	28	58	rVB2	19614	46461	4.98%	0.583%
2	1.599	83	96	105	rBV2	161624	296271	31.76%	3.719%
3	1.914	187	194	210	rVB	105027	145161	15.56%	1.822%
4	2.567	383	397	412	rVB	148660	246327	26.41%	3.092%
5	4.631	1024	1039	1073	rBV	138186	419152	44.94%	5.262%
6	5.062	1154	1173	1189	rBV2	178052	398267	42.70%	5.000%
7	5.721	1358	1378	1399	rBV2	345016	904833	97.01%	11.359%
8	6.248	1528	1542	1564	rBV2	321758	637961	68.39%	8.009%
9	6.689	1663	1679	1697	rBV	229599	455589	48.84%	5.719%
10	7.563	1938	1951	1974	rBV	86668	165575	17.75%	2.079%
11	7.894	2041	2054	2073	rBV	388153	697552	74.78%	8.757%
12	8.181	2131	2143	2165	rBV	55604	99304	10.65%	1.247%
13	8.634	2272	2284	2319	rBV2	450276	932767	100.00%	11.709%
14	9.415	2514	2527	2556	rBV	463804	793943	85.12%	9.967%
15	10.753	2931	2943	2961	rBV	163324	271644	29.12%	3.410%
16	11.811	3259	3272	3289	rBV	463400	754774	80.92%	9.475%
17	12.190	3378	3390	3409	rBV	384732	644963	69.15%	8.096%
18	13.846	3893	3905	3912	rBV3	7187	11541	1.24%	0.145%
19	14.335	4047	4057	4063	rBV6	6763	10751	1.15%	0.135%
20	16.881	4841	4849	4858	rBV2	23226	33153	3.55%	0.416%




Sum of corrected areas: 7965989

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061523\
Data File : VU054538.D
Acq On : 15 Jun 2023 21:06
Operator : MD/SY
Sample : 03253-13
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXYW6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

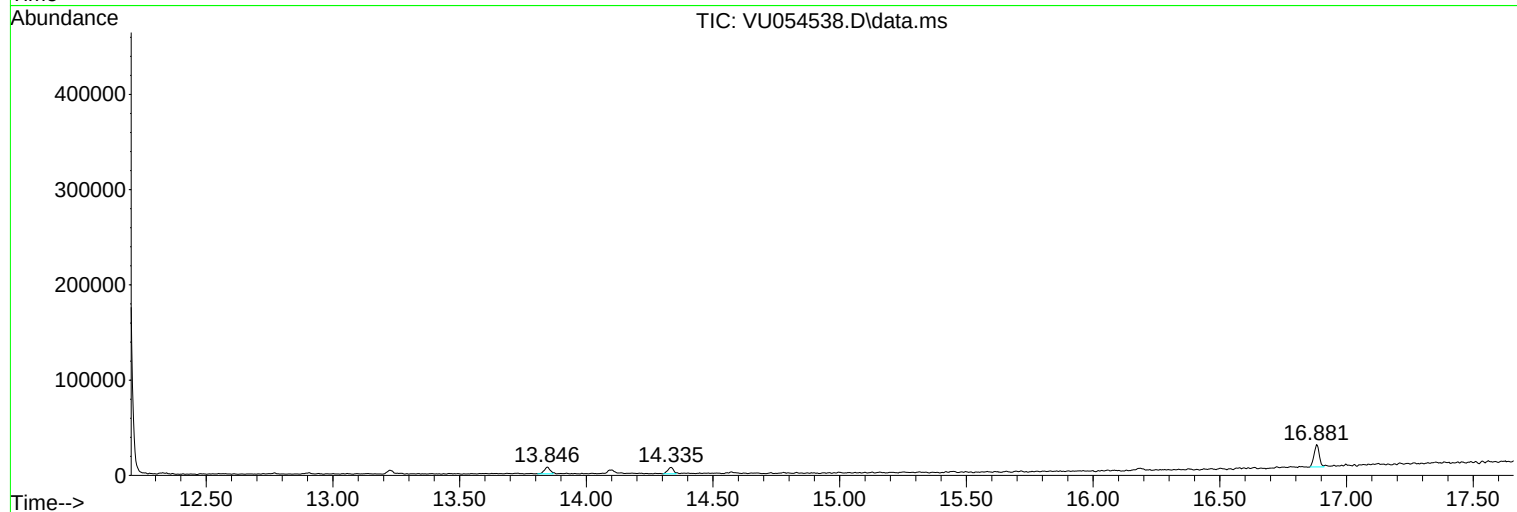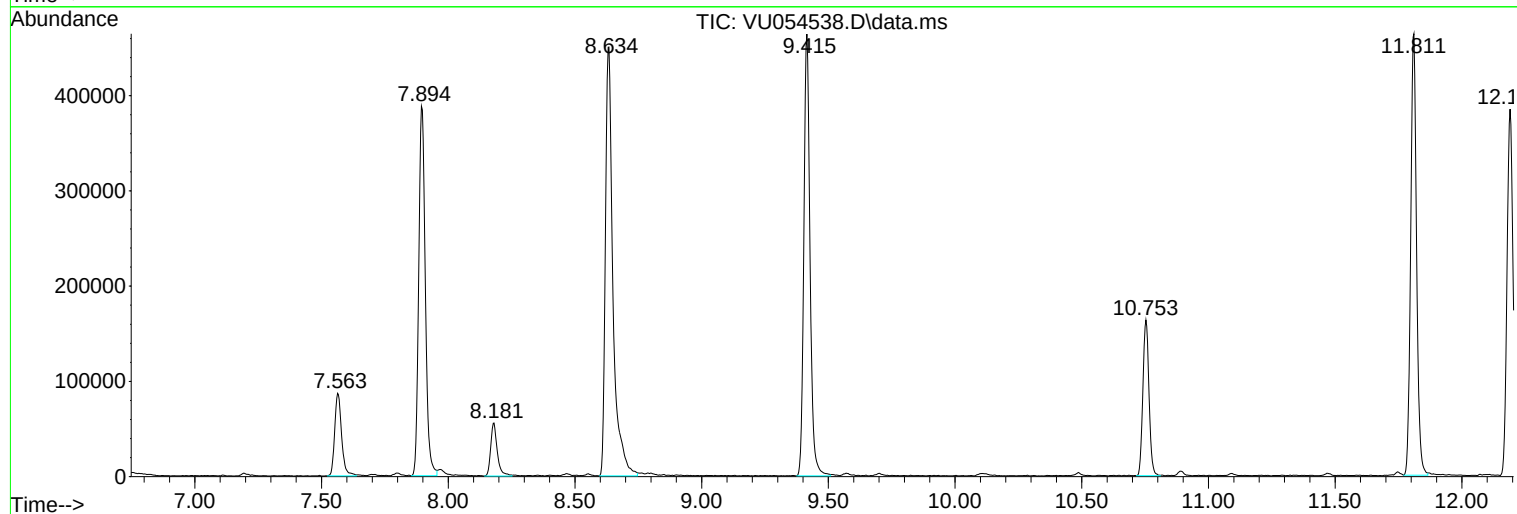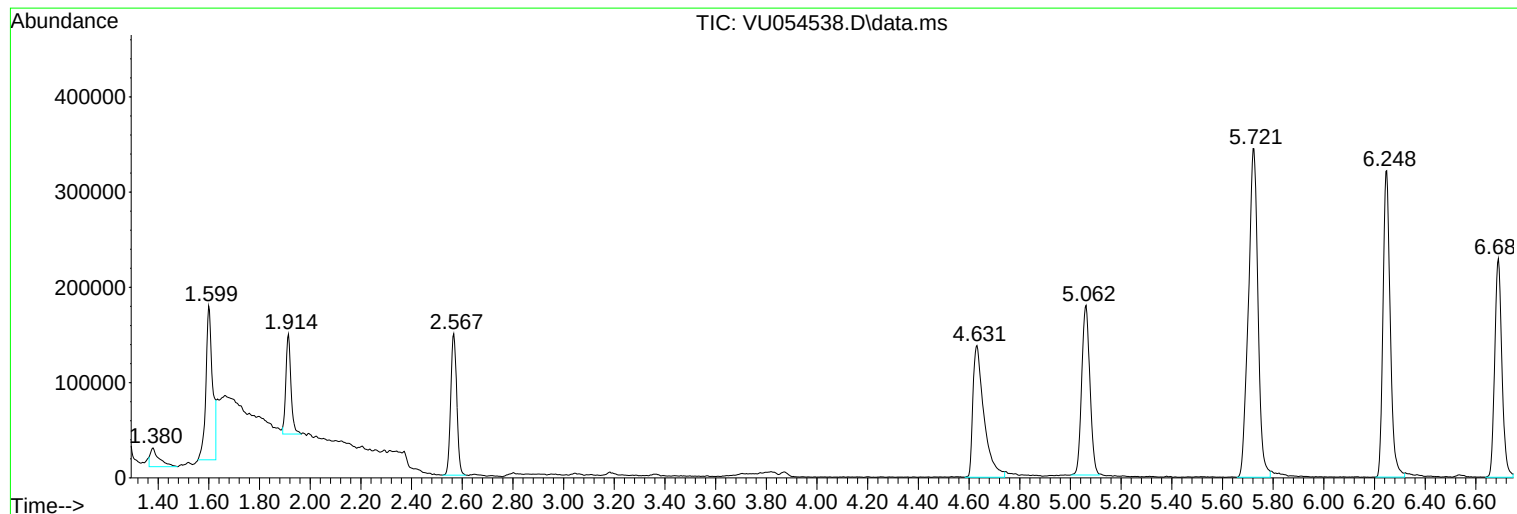

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061523\
Data File : VU054538.D
Acq On : 15 Jun 2023 21:06
Operator : MD/SY
Sample : 03253-13
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXYW6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061523\
Data File : VU054538.D
Acq On : 15 Jun 2023 21:06
Operator : MD/SY
Sample : 03253-13
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXYW6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc