

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061523\
 Data File : VU054541.D
 Acq On : 15 Jun 2023 22:18
 Operator : MD/SY
 Sample : 03253-16
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXYX1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU054541.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.499	56	65	82	rBV2	43858	148109	15.73%	1.789%
2	1.599	89	96	111	rVB	81995	99600	10.58%	1.203%
3	1.914	186	194	212	rVB	100195	141906	15.07%	1.714%
4	2.566	384	397	413	rBV2	147907	248867	26.44%	3.006%
5	3.357	631	643	659	rBV3	14434	34241	3.64%	0.414%
6	3.869	788	802	816	rBV2	33903	78212	8.31%	0.945%
7	4.660	1025	1048	1076	rBV3	164147	653433	69.41%	7.892%
8	5.061	1156	1173	1198	rVB	176336	416924	44.29%	5.035%
9	5.315	1238	1252	1266	rVB3	12459	25801	2.74%	0.312%
10	5.721	1354	1378	1396	rBV2	341450	892280	94.78%	10.777%
11	6.245	1528	1541	1573	rBV	312702	623973	66.28%	7.536%
12	6.544	1623	1634	1648	rVB3	24489	46558	4.95%	0.562%
13	6.688	1665	1679	1702	rBV	222843	454249	48.25%	5.486%
14	7.563	1939	1951	1973	rBV	87092	162602	17.27%	1.964%
15	7.894	2038	2054	2075	rBV	385753	687826	73.06%	8.307%
16	8.177	2132	2142	2158	rBV	52682	95727	10.17%	1.156%
17	8.550	2249	2258	2270	rBV3	19870	34129	3.63%	0.412%
18	8.630	2270	2283	2323	rBV2	463885	941406	100.00%	11.370%
19	9.415	2514	2527	2555	rBV	447489	767161	81.49%	9.265%
20	9.698	2605	2615	2623	rBV4	7516	13129	1.39%	0.159%
21	10.753	2931	2943	2960	rBV2	168703	291756	30.99%	3.524%
22	10.891	2975	2986	2998	rBV2	11558	19544	2.08%	0.236%
23	11.807	3259	3271	3296	rBV	449857	737709	78.36%	8.910%
24	12.068	3342	3352	3367	rBV2	15321	35024	3.72%	0.423%
25	12.190	3378	3390	3411	rVB	375570	629681	66.89%	7.605%




Sum of corrected areas: 8279847

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061523\
Data File : VU054541.D
Acq On : 15 Jun 2023 22:18
Operator : MD/SY
Sample : 03253-16
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXYX1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

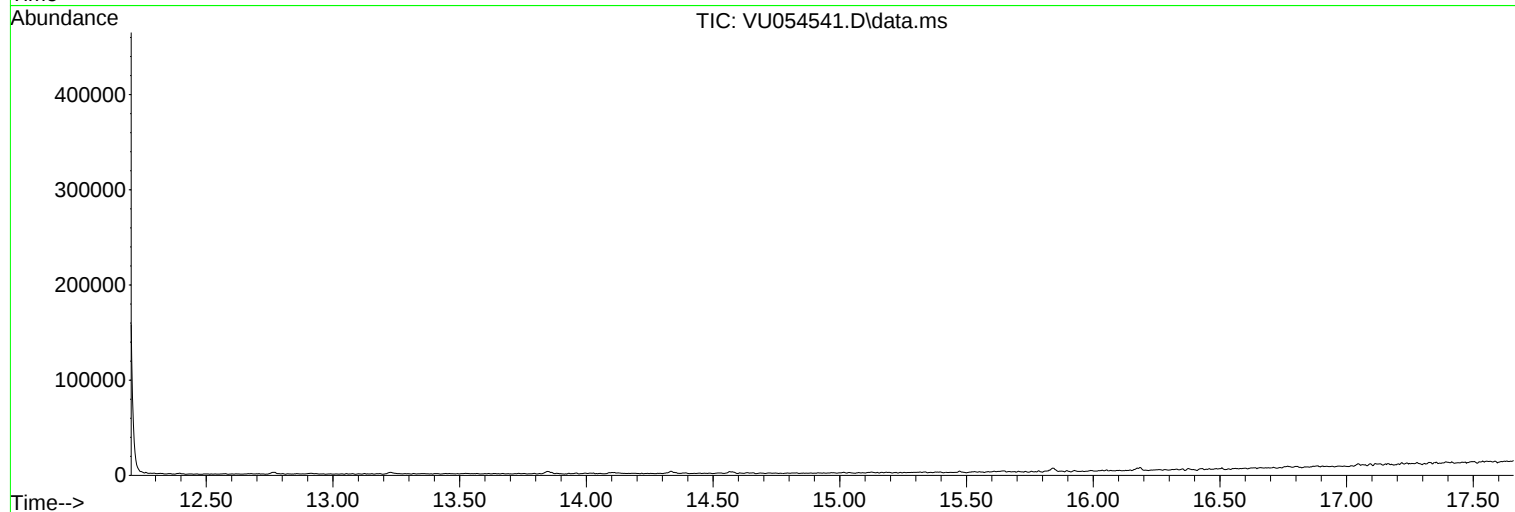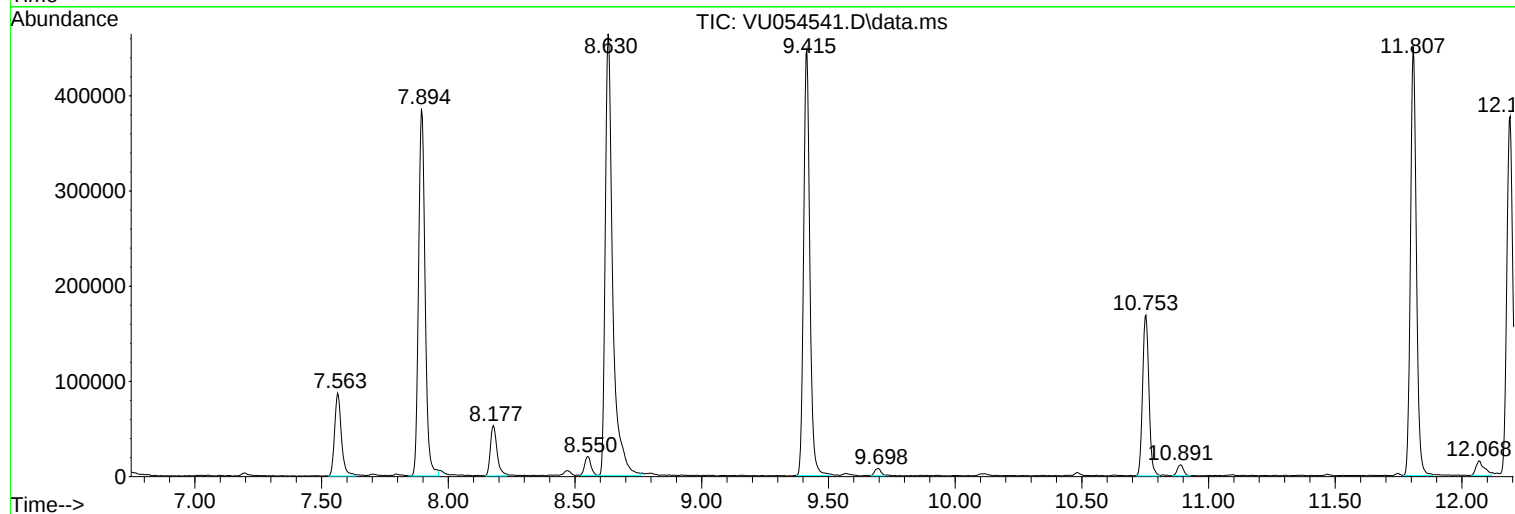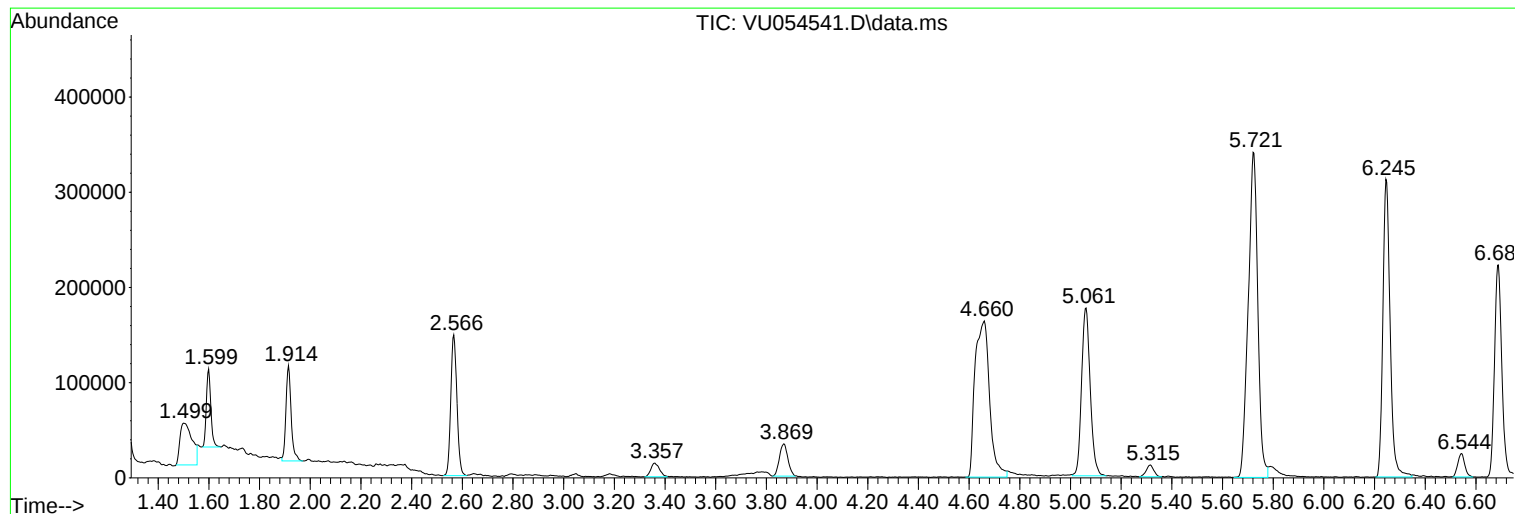

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061523\
Data File : VU054541.D
Acq On : 15 Jun 2023 22:18
Operator : MD/SY
Sample : 03253-16
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXYX1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061523\
Data File : VU054541.D
Acq On : 15 Jun 2023 22:18
Operator : MD/SY
Sample : 03253-16
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXYX1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------