

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061523\
 Data File : VU054549.D
 Acq On : 16 Jun 2023 01:33
 Operator : MD/SY
 Sample : 03232-10
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 CONR6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU054549.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	89	96	114	rVB	74541	90239	10.13%	1.234%
2	1.914	186	194	206	rBV	93684	125457	14.08%	1.716%
3	2.566	385	397	413	rBV	136991	222969	25.02%	3.049%
4	4.631	1028	1039	1071	rBV	124132	375458	42.14%	5.135%
5	5.058	1157	1172	1192	rVB	169730	374171	41.99%	5.117%
6	5.721	1355	1378	1404	rBV2	328027	863723	96.93%	11.812%
7	6.245	1528	1541	1564	rBV	313417	618752	69.44%	8.462%
8	6.685	1664	1678	1696	rBV	213265	423864	47.57%	5.797%
9	7.563	1938	1951	1974	rBV2	79823	151029	16.95%	2.065%
10	7.894	2041	2054	2072	rBV	361530	645870	72.48%	8.833%
11	8.177	2132	2142	2162	rBV2	48659	85905	9.64%	1.175%
12	8.467	2220	2232	2244	rBV2	5770	11698	1.31%	0.160%
13	8.630	2272	2283	2324	rBV2	432392	891072	100.00%	12.186%
14	9.415	2511	2527	2549	rBV	437156	755419	84.78%	10.331%
15	10.753	2930	2943	2960	rBV	155543	256823	28.82%	3.512%
16	10.891	2971	2986	2996	rVB2	12060	18906	2.12%	0.259%
17	11.807	3259	3271	3299	rBV	436990	724784	81.34%	9.912%
18	12.064	3340	3351	3375	rBV3	25859	68495	7.69%	0.937%
19	12.190	3378	3390	3417	rVB	370852	607700	68.20%	8.311%




Sum of corrected areas: 7312334

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061523\
Data File : VU054549.D
Acq On : 16 Jun 2023 01:33
Operator : MD/SY
Sample : 03232-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
CONR6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

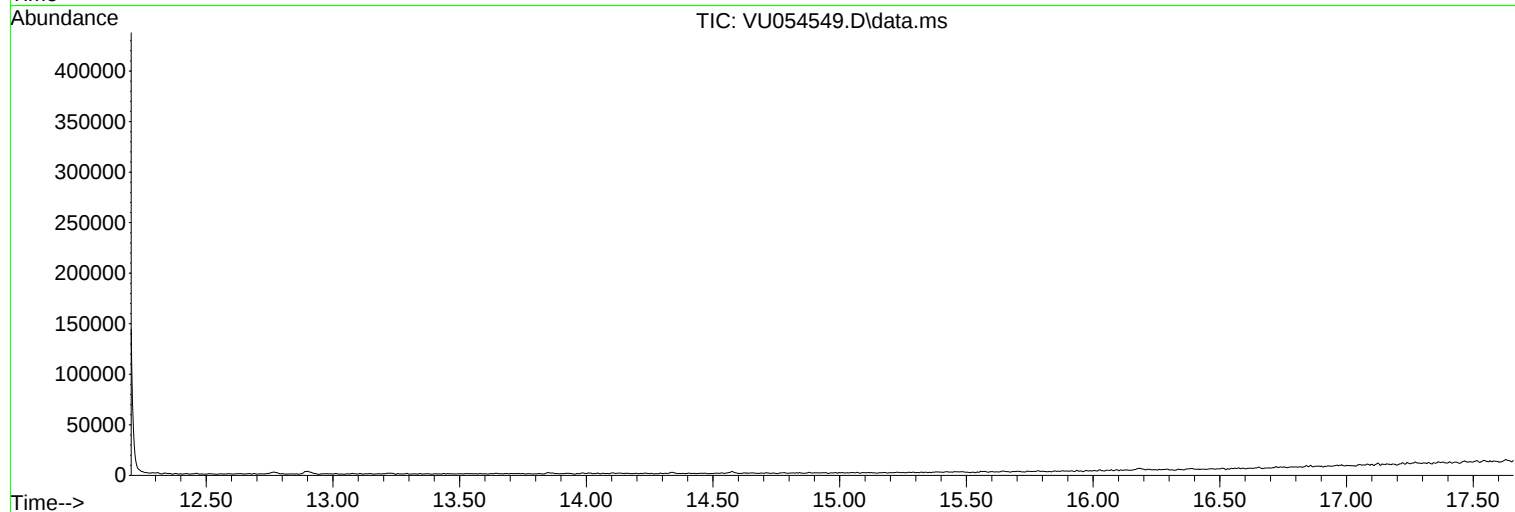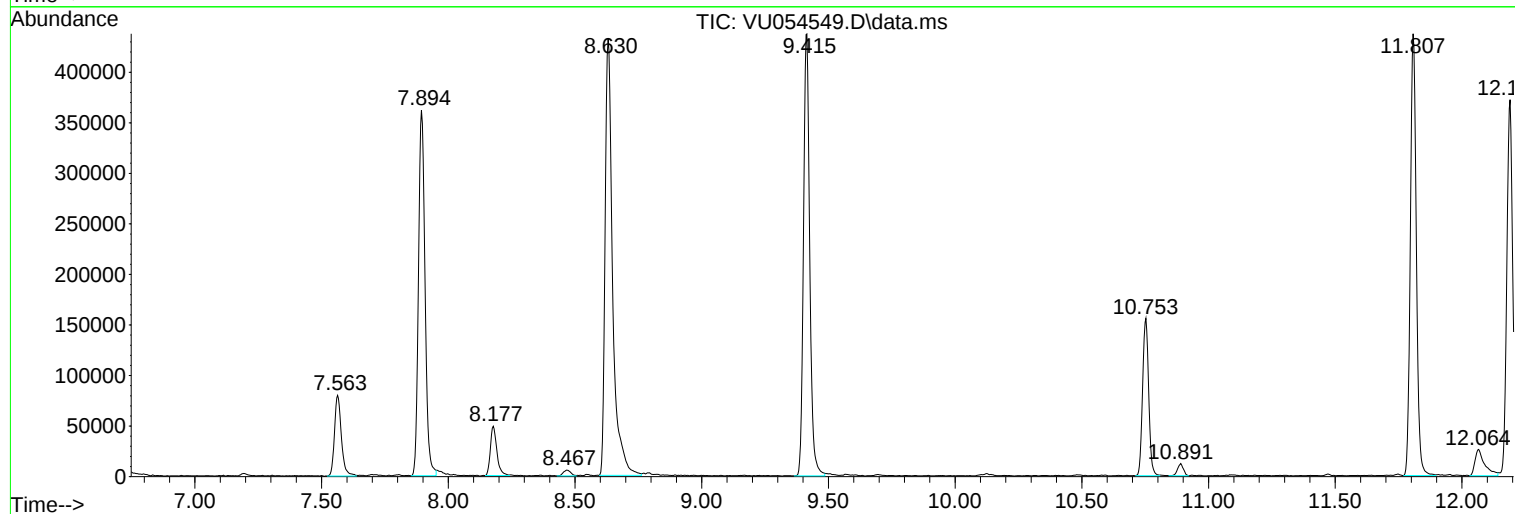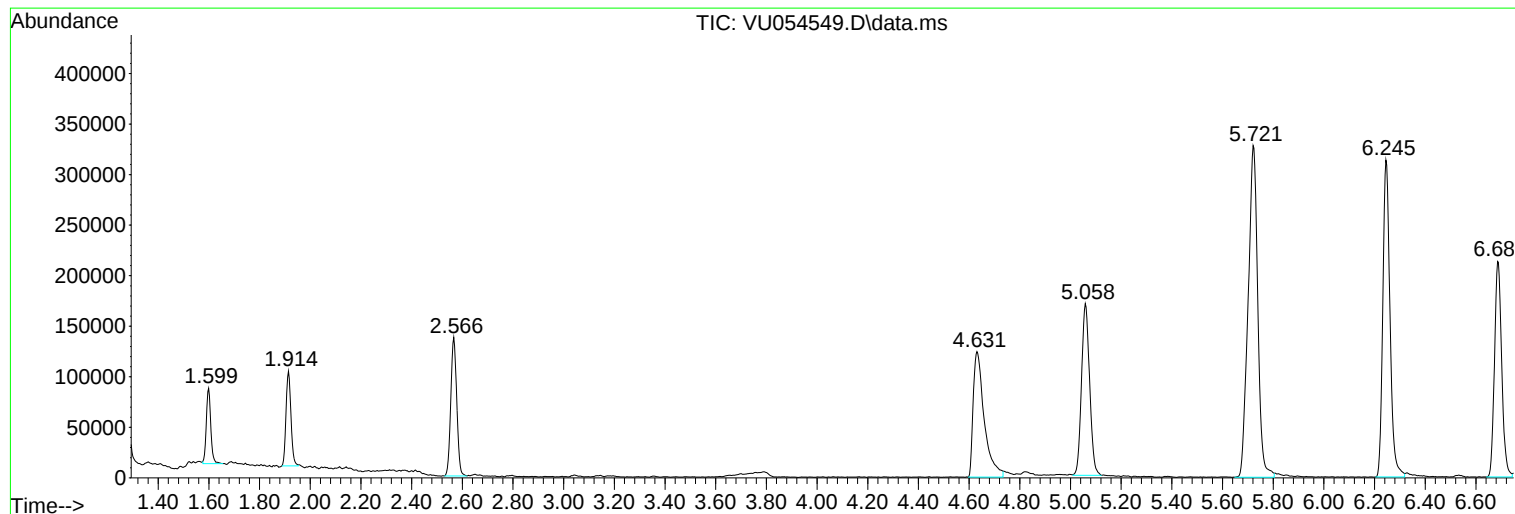

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061523\
Data File : VU054549.D
Acq On : 16 Jun 2023 01:33
Operator : MD/SY
Sample : 03232-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
CONR6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061523\
Data File : VU054549.D
Acq On : 16 Jun 2023 01:33
Operator : MD/SY
Sample : 03232-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
CONR6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------