

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061523\
 Data File : VU054556.D
 Acq On : 16 Jun 2023 04:22
 Operator : MD/SY
 Sample : 03232-07
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 CONR3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU054556.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	89	96	108	rVB	79005	92150	10.18%	1.245%
2	1.914	186	194	207	rVB	99987	132320	14.61%	1.788%
3	2.566	385	397	415	rBV	137753	227482	25.12%	3.073%
4	4.631	1026	1039	1080	rBV	125597	383386	42.34%	5.179%
5	5.058	1156	1172	1193	rVB2	167666	379316	41.89%	5.124%
6	5.721	1358	1378	1405	rBV2	322895	868576	95.92%	11.734%
7	6.245	1527	1541	1572	rBV	310100	620591	68.53%	8.384%
8	6.537	1622	1632	1644	rBV8	8054	16382	1.81%	0.221%
9	6.685	1664	1678	1710	rBV	215519	436841	48.24%	5.902%
10	7.563	1939	1951	1969	rBV	80220	149700	16.53%	2.022%
11	7.894	2037	2054	2073	rBV	369220	651780	71.98%	8.805%
12	8.177	2131	2142	2160	rBV	50303	89428	9.88%	1.208%
13	8.631	2270	2283	2317	rBV2	437098	905518	100.00%	12.233%
14	9.415	2514	2527	2550	rBV	439854	765360	84.52%	10.340%
15	10.753	2930	2943	2959	rBV	156590	263011	29.05%	3.553%
16	10.891	2976	2986	2995	rVB2	6714	11100	1.23%	0.150%
17	11.807	3259	3271	3288	rBV	445052	725486	80.12%	9.801%
18	12.061	3341	3350	3374	rBV2	29685	75426	8.33%	1.019%
19	12.190	3378	3390	3413	rVB	358581	608247	67.17%	8.217%




Sum of corrected areas: 7402100

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061523\
Data File : VU054556.D
Acq On : 16 Jun 2023 04:22
Operator : MD/SY
Sample : 03232-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
CONR3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

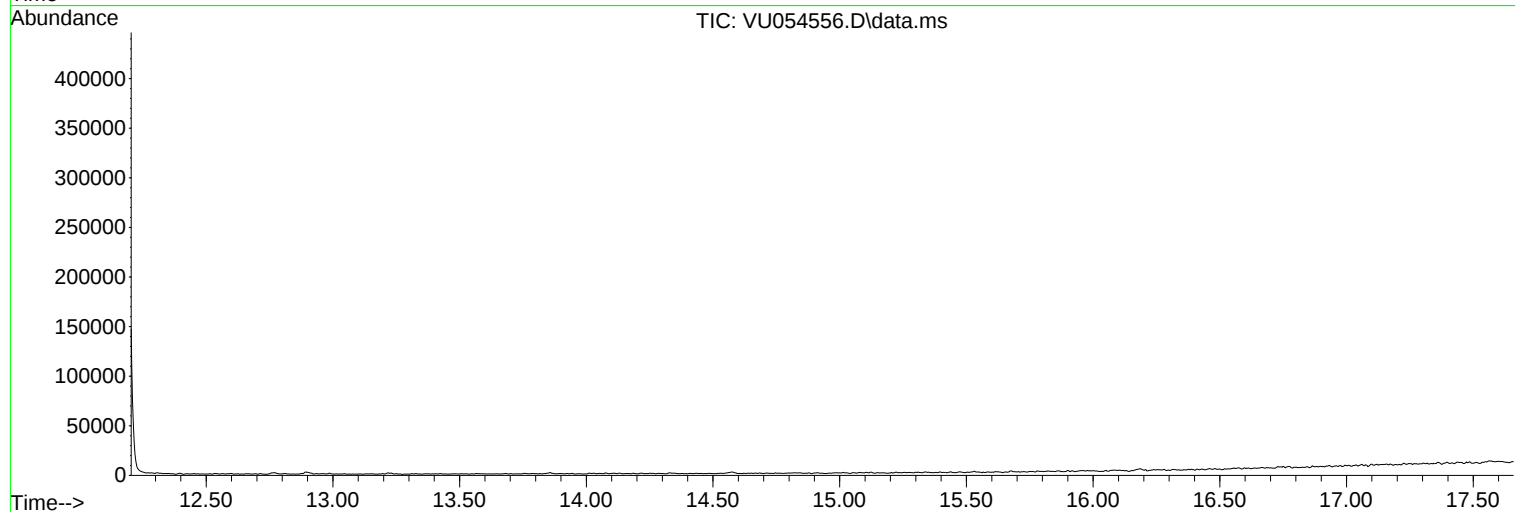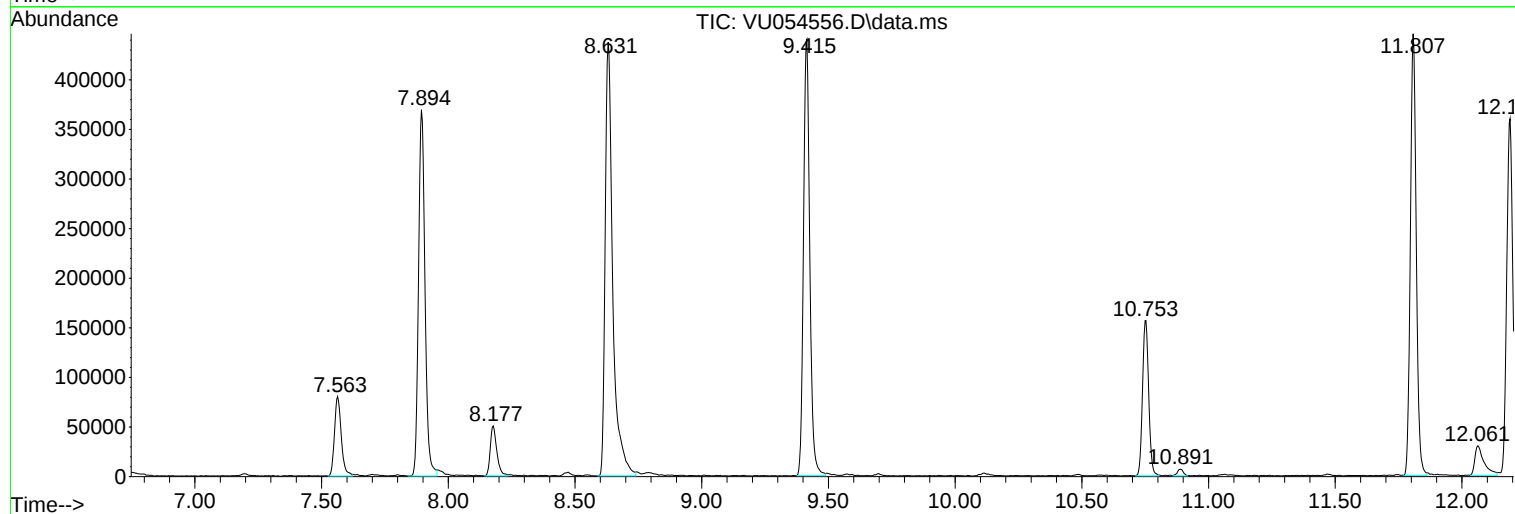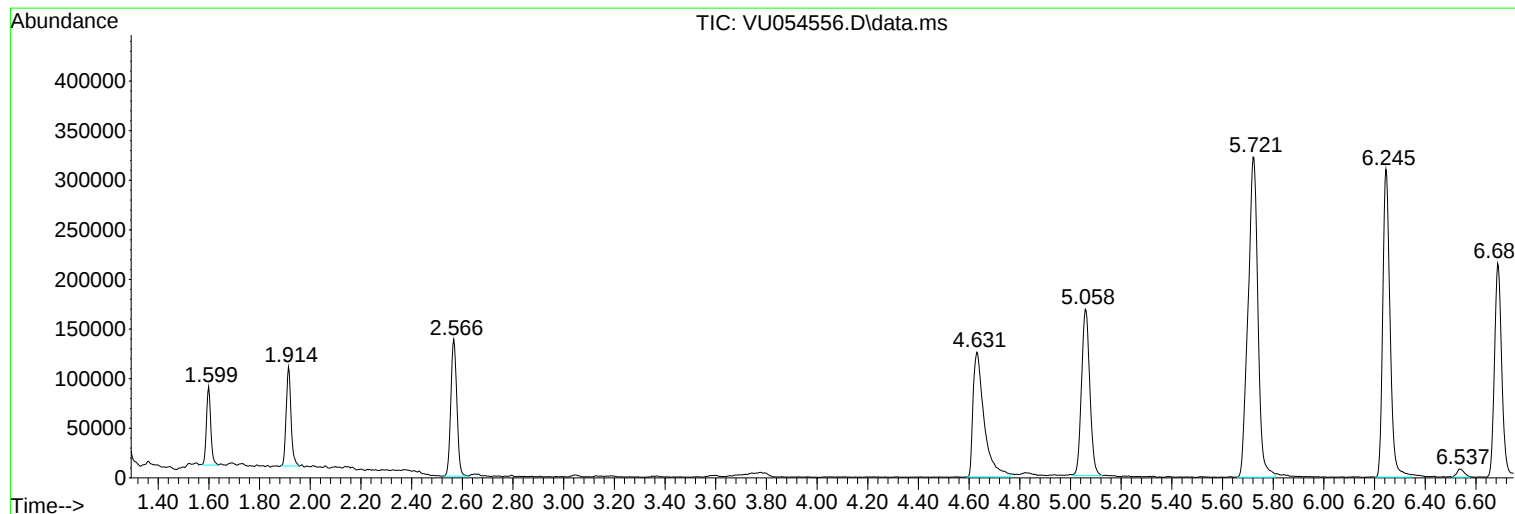

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061523\
Data File : VU054556.D
Acq On : 16 Jun 2023 04:22
Operator : MD/SY
Sample : 03232-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
CONR3










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 1-Hexanol, 2-ethyl- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
12.061	0.52 ug/L	75426	1,4-Dichlorobenzene-d4	11.807

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			1-Hexanol, 2-ethyl-	130	C8H18O	000104-76-7	86
2			1-Hexanol, 2-ethyl-	130	C8H18O	000104-76-7	64
3			1-Hexanol, 2-ethyl-	130	C8H18O	000104-76-7	53
4			1-Pentanol, 2-ethyl-4-methyl-	130	C8H18O	000106-67-2	47
5			2-Propyl-1-pentanol, chlorodiflu...	242	C10H17ClF2O2	1000447-27-3	47

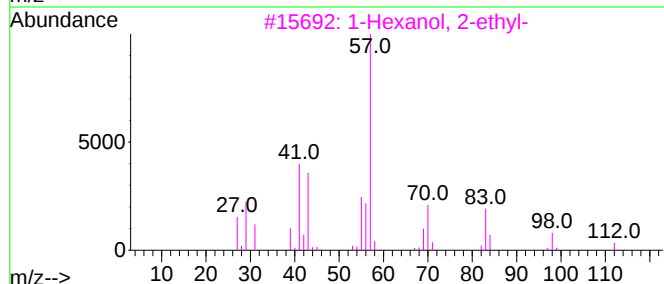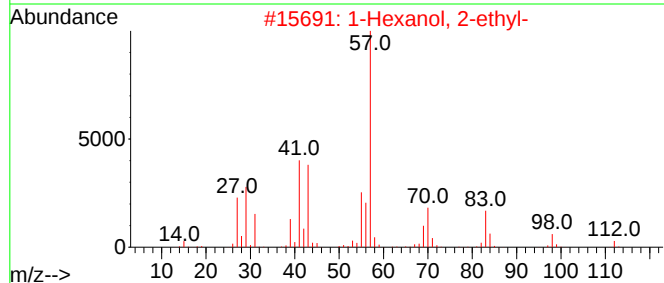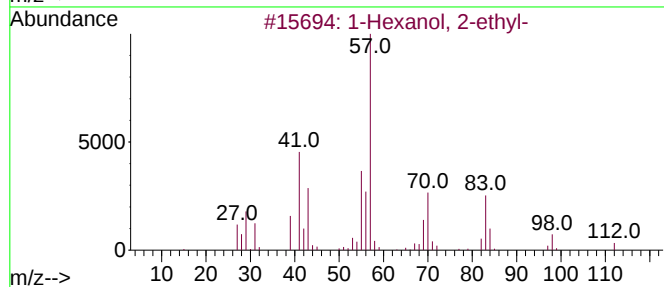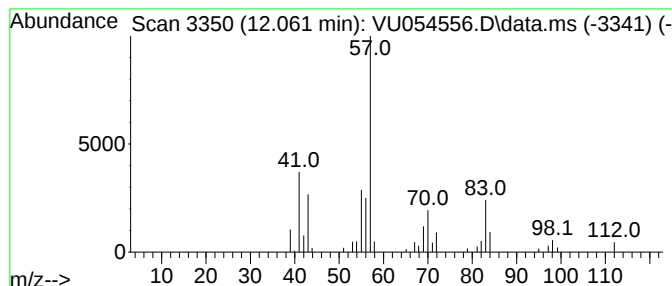

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061523\
Data File : VU054556.D
Acq On : 16 Jun 2023 04:22
Operator : MD/SY
Sample : 03232-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
CONR3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
1-Hexanol, 2-et...	12.061	0.5	ug/L	75426	3	11.807	725486	5.0