


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061523\
 Data File : VU054512.D
 Acq On : 15 Jun 2023 08:54
 Operator : MD/SY
 Sample : BFB019
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB019

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Sat Jun 17 06:10:25 2023

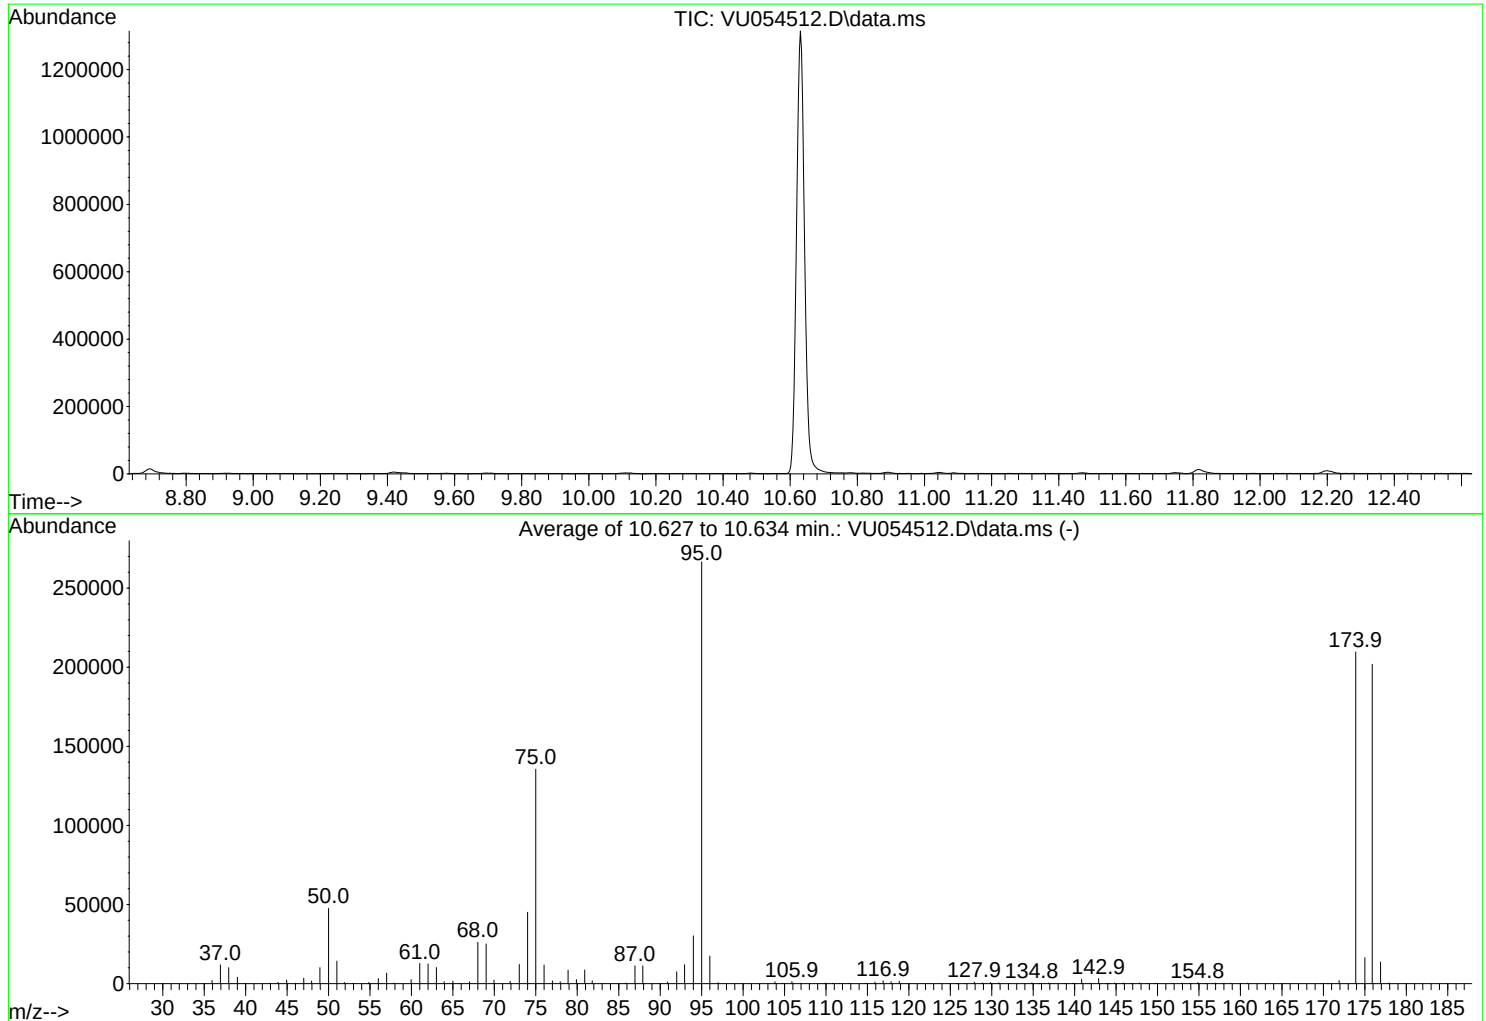

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	47581	PASS
75	95	30	80	50.8	135509	PASS
95	95	100	100	100.0	266581	PASS
96	95	5	9	6.5	17452	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	78.6	209600	PASS
175	174	5	9	7.9	16538	PASS
176	174	95	101	96.3	201899	PASS
177	176	5	9	6.8	13670	PASS

m/z	Abundance
39.80	205.0
40.80	101.0
43.90	813.0

Instrument :
MSVOA_U
ClientSampleId :
BFB019

m/z	Abundance
35.90	2105.0
36.90	12087.0
37.90	10300.0
39.00	4174.0
39.90	465.0
42.90	201.0
44.00	1559.0
45.00	2271.0
46.00	292.0
47.00	3574.0
48.00	1714.0
48.90	10197.0
50.00	47528.0
51.00	14191.0
51.90	724.0
52.90	197.0
54.90	752.0
56.00	3392.0
57.00	6656.0
57.90	337.0
60.00	2556.0
61.00	12671.0
62.00	12816.0
63.00	9989.0
64.00	1255.0
65.00	1591.0
65.80	165.0
67.00	915.0
68.00	26224.0
69.00	25240.0
69.90	2049.0
71.90	1536.0
73.00	11946.0
74.00	45152.0
75.00	134784.0
76.00	11894.0
77.00	1530.0
77.90	1353.0
78.90	8276.0
79.90	2548.0
80.90	8485.0
81.80	1791.0
82.80	168.0
85.80	330.0
86.90	10956.0
87.90	11304.0
90.90	1019.0
92.00	7413.0
93.00	12563.0
94.00	30592.0
95.00	264000.0
96.00	18040.0
97.00	551.0
103.80	1274.0
104.90	305.0
105.90	1184.0
107.00	178.0
109.90	340.0
110.80	323.0
111.60	192.0
112.90	210.0
114.80	305.0
115.90	1126.0
116.90	1861.0
117.90	1143.0
118.80	1542.0
123.80	166.0
127.90	1009.0
128.90	417.0
129.80	783.0
130.80	523.0
134.90	595.0
136.90	394.0
138.80	159.0
139.90	258.0
140.90	2675.0
141.80	336.0
142.90	3160.0
143.90	240.0
144.80	571.0
145.90	394.0
146.80	144.0
147.80	573.0
148.80	180.0
149.70	273.0
151.70	157.0
152.90	275.0
154.00	194.0
154.80	646.0
155.90	177.0
156.90	489.0
158.80	262.0

Instrument :
MSVOA_U
ClientSampleId :
BFB019

160.90	303.0
169.70	142.0
170.50	142.0
171.00	362.0
171.90	1910.0
173.90	202304.0
175.00	16504.0
175.90	193216.0
176.90	13180.0
177.90	525.0

Instrument :
MSVOA_U
ClientSampleId :
BFB019

m/z	Abundance
36.00	2069.0
37.00	12184.0
37.90	10304.0
39.00	4126.0
39.90	439.0
42.90	215.0
43.90	1662.0
44.90	2389.0
46.10	337.0
47.00	3641.0
47.90	1559.0
48.90	10507.0
50.00	48920.0
51.00	14756.0
51.90	766.0
52.90	251.0
54.90	752.0
56.00	3348.0
57.00	6858.0
57.80	322.0
59.90	2561.0
61.00	13129.0
62.00	12734.0
63.00	10672.0
63.90	1262.0
65.00	1710.0
65.80	162.0
67.00	1141.0
68.00	27024.0
69.00	25560.0
70.00	2372.0
71.90	1624.0
73.00	12625.0
74.00	46616.0
75.00	139904.0
76.00	11981.0
77.00	1780.0
77.90	1223.0
78.90	8678.0
79.90	2621.0
80.90	8874.0
81.80	1889.0
82.80	164.0
85.90	499.0
87.00	11535.0
87.90	11562.0
90.90	1084.0
92.00	7836.0
93.00	12353.0
94.00	30904.0
95.00	274368.0
96.00	18128.0
97.00	598.0
103.90	1276.0
104.70	318.0
105.90	1304.0
106.90	241.0
109.90	295.0
110.80	389.0
111.90	196.0
112.70	186.0
114.80	268.0
115.90	1069.0
116.90	1930.0
117.80	1263.0
118.90	1512.0
123.70	139.0
125.80	101.0
126.70	103.0
127.90	1035.0
128.80	402.0
129.90	753.0
130.90	530.0
134.80	566.0
136.90	380.0
138.80	171.0
139.80	285.0
140.90	2750.0
141.90	363.0
142.90	3329.0
143.90	207.0
144.80	542.0
145.90	416.0
147.80	558.0
148.80	191.0
149.80	297.0
151.70	146.0
152.90	295.0
153.90	189.0
154.90	695.0
155.80	155.0
156.90	435.0

Instrument :
MSVOA_U
ClientSampleId :
BFB019

158.80	319.0
160.80	344.0
169.70	174.0
171.00	363.0
171.90	2059.0
173.90	215488.0
175.00	17056.0
175.90	208192.0
176.90	14067.0
177.90	449.0

Instrument :
MSVOA_U
ClientSampleId :
BFB019

m/z	Abundance
36.00	1925.0
37.00	11167.0
38.00	9671.0
39.00	4026.0
39.90	399.0
42.90	212.0
43.90	1804.0
44.90	2163.0
46.10	287.0
47.00	3259.0
47.90	1489.0
49.00	9677.0
50.00	46296.0
51.00	14009.0
51.90	730.0
52.90	268.0
54.80	706.0
56.00	3134.0
57.00	6663.0
57.90	227.0
59.90	2396.0
61.00	12534.0
62.00	11834.0
63.00	10049.0
63.90	1198.0
65.00	1669.0
65.90	160.0
67.00	1178.0
68.00	25512.0
69.00	24496.0
70.00	2347.0
71.90	1557.0
73.00	11785.0
74.00	43480.0
75.00	131840.0
76.00	11387.0
77.00	1789.0
78.00	1108.0
78.90	8409.0
79.90	2319.0
80.90	8520.0
81.80	1698.0
82.90	138.0
85.90	532.0
87.00	11489.0
87.90	10890.0
90.90	1039.0
92.00	7233.0
92.90	11075.0
94.00	29408.0
95.00	261376.0
96.00	16189.0
97.00	532.0
103.90	1181.0
104.70	405.0
105.90	1366.0
106.90	245.0
109.90	234.0
110.80	318.0
112.00	199.0
112.70	167.0
114.80	223.0
115.90	974.0
116.90	1824.0
117.80	1212.0
118.90	1485.0
123.70	102.0
126.70	105.0
127.90	920.0
128.80	386.0
129.90	680.0
130.90	415.0
134.90	478.0
135.70	119.0
136.80	401.0
138.80	128.0
139.70	299.0
140.80	2770.0
141.90	382.0
142.90	3213.0
144.10	185.0
144.80	447.0
145.80	398.0
147.80	547.0
148.70	160.0
149.80	302.0
151.80	108.0
152.90	236.0
153.80	167.0
154.90	712.0
155.70	113.0
157.00	435.0

Instrument :
MSVOA_U
ClientSampleId :
BFB019

157.90	109.0
158.80	371.0
160.80	306.0
169.70	132.0
171.90	1951.0
173.90	211008.0
175.00	16054.0
175.90	204288.0
176.90	13764.0
177.90	397.0

Instrument :
MSVOA_U
ClientSampleId :
BFB019