

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU061621\  
 Data File : VU044237.D  
 Acq On : 16 Jun 2021 13:47  
 Operator : SY/MD  
 Sample : VIBLK  
 Misc : 5.0mL/MSVOA\_U/WATER  
 ALS Vial : 10 Sample Multiplier: 1

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 VIBLK

Integration Parameters: RTEINT.P

Integrator: RTE

Smoother: ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\82U060921W.M

Title : SW846 8260

Signal : TIC: VU044237.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 4.658       | 1011          | 1032        | 1048         | rBV2     | 6432           | 21144         | 1.67%           | 0.297%        |
| 2         | 5.298       | 1214          | 1231        | 1244         | rBV      | 186835         | 397661        | 31.47%          | 5.584%        |
| 3         | 5.382       | 1244          | 1257        | 1276         | rVB      | 333605         | 683573        | 54.10%          | 9.598%        |
| 4         | 5.713       | 1344          | 1360        | 1384         | rBV      | 205219         | 422959        | 33.48%          | 5.939%        |
| 5         | 6.256       | 1515          | 1529        | 1556         | rBV      | 471218         | 886130        | 70.14%          | 12.442%       |
| 6         | 7.906       | 2028          | 2042        | 2064         | rBV      | 742168         | 1263450       | 100.00%         | 17.740%       |
| 7         | 9.423       | 2500          | 2514        | 2549         | rBV      | 660479         | 1094310       | 86.61%          | 15.365%       |
| 8         | 10.639      | 2879          | 2892        | 2918         | rVB      | 545528         | 866404        | 68.57%          | 12.165%       |
| 9         | 11.475      | 3140          | 3152        | 3168         | rBV      | 54968          | 101214        | 8.01%           | 1.421%        |
| 10        | 11.819      | 3246          | 3259        | 3277         | rBV      | 761358         | 1209354       | 95.72%          | 16.980%       |
| 11        | 12.822      | 3559          | 3571        | 3580         | rBV      | 9466           | 15760         | 1.25%           | 0.221%        |
| 12        | 15.224      | 4307          | 4318        | 4330         | rVB      | 5652           | 13130         | 1.04%           | 0.184%        |
| 13        | 15.410      | 4362          | 4376        | 4384         | rBV5     | 13087          | 21187         | 1.68%           | 0.297%        |
| 14        | 15.986      | 4548          | 4555        | 4565         | rVB4     | 13618          | 21635         | 1.71%           | 0.304%        |
| 15        | 16.301      | 4646          | 4653        | 4663         | rVB      | 30920          | 44107         | 3.49%           | 0.619%        |
| 16        | 16.892      | 4831          | 4837        | 4842         | rBV9     | 8398           | 13599         | 1.08%           | 0.191%        |
| 17        | 17.143      | 4908          | 4915        | 4925         | rVB2     | 31279          | 46455         | 3.68%           | 0.652%        |


Sum of corrected areas: 7122072

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU061621\  
Data File : VU044237.D  
Acq On : 16 Jun 2021 13:47  
Operator : SY/MD  
Sample : VIBLK  
Misc : 5.0mL/MSVOA\_U/WATER  
ALS Vial : 10 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\82U060921W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

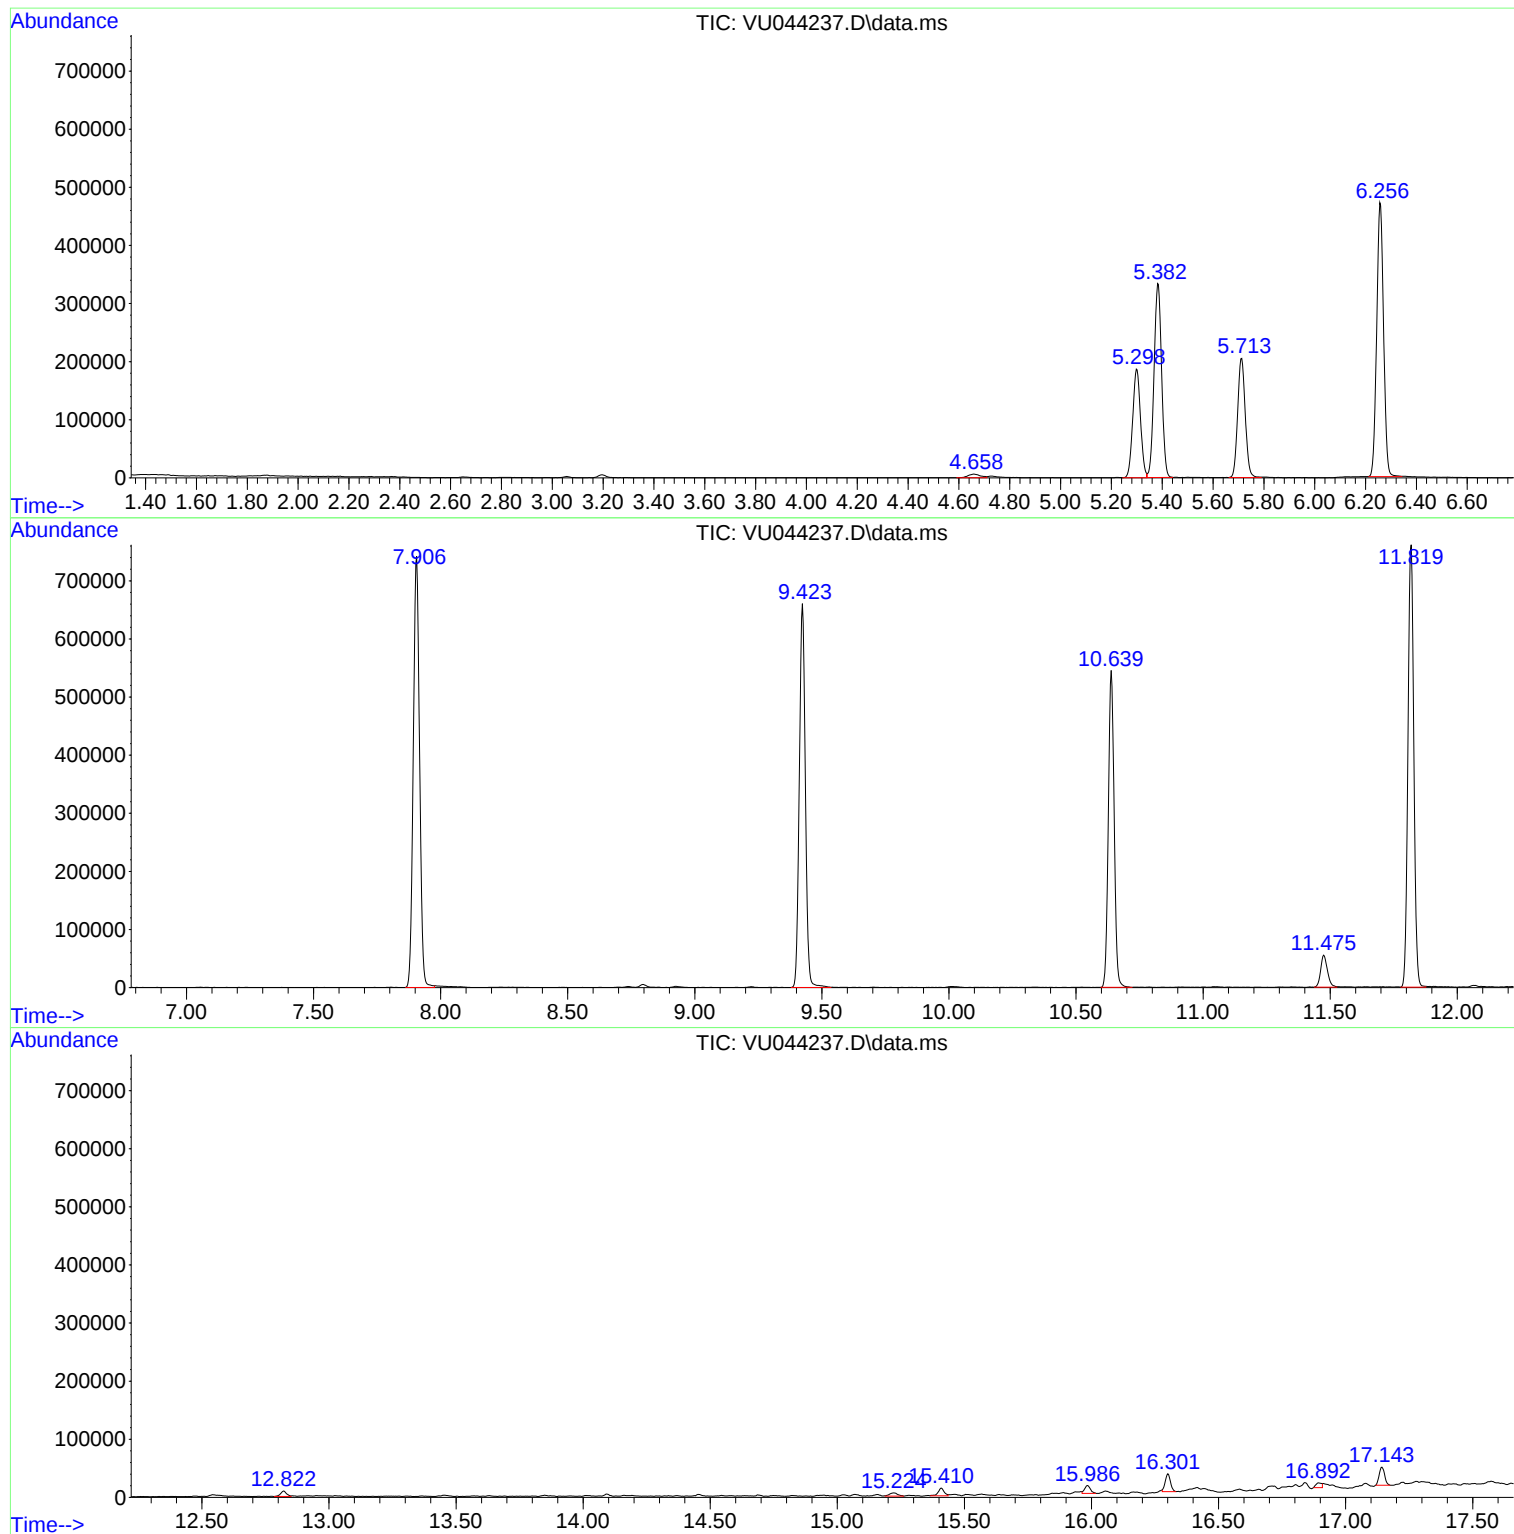

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU061621\  
Data File : VU044237.D  
Acq On : 16 Jun 2021 13:47  
Operator : SY/MD  
Sample : VIBLK  
Misc : 5.0mL/MSVOA\_U/WATER  
ALS Vial : 10 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\82U060921W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU061621\  
Data File : VU044237.D  
Acq On : 16 Jun 2021 13:47  
Operator : SY/MD  
Sample : VIBLK  
Misc : 5.0mL/MSVOA\_U/WATER  
ALS Vial : 10 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\82U060921W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |    |      |      |
|------------------|----|---------|-------|----------|-----------------------|----|------|------|
|                  |    |         |       |          | #                     | RT | Resp | Conc |

-----