


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061621\
Data File : VU044229.D
Acq On : 16 Jun 2021 09:11
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U060921W.M
Title : SW846 8260
Last Update : Thu Jun 10 05:11:37 2021

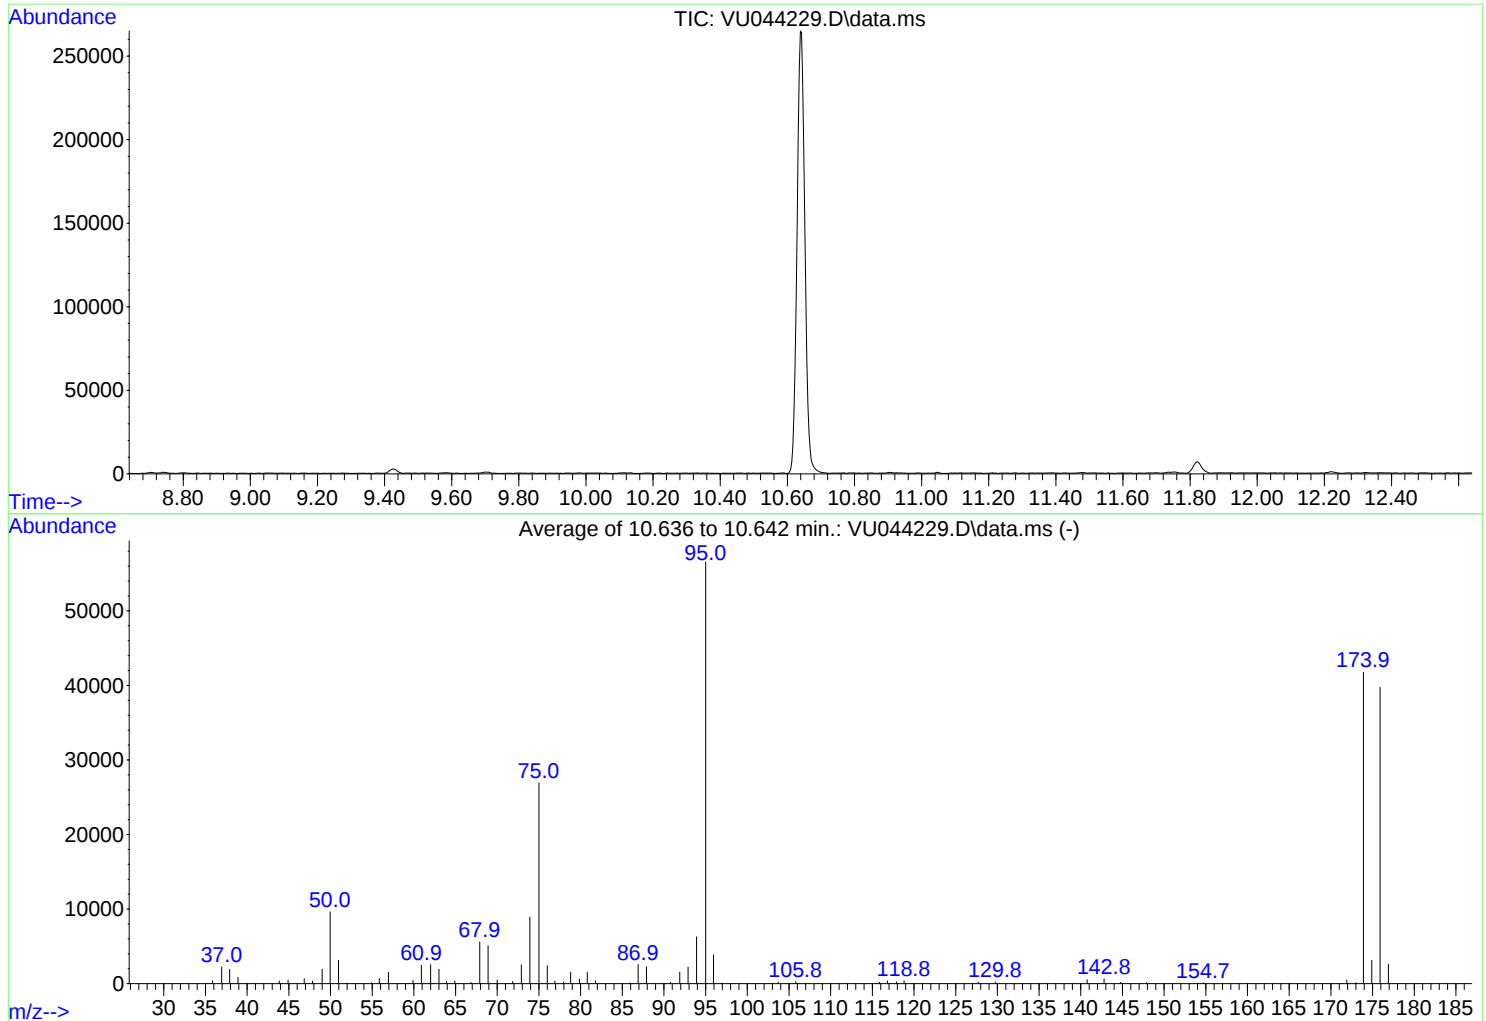

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	9634	PASS
75	95	30	60	47.6	26928	PASS
95	95	100	100	100.0	56576	PASS
96	95	5	9	6.8	3854	PASS
173	174	0.00	2	0.3	141	PASS
174	95	50	100	73.8	41744	PASS
175	174	5	9	7.5	3140	PASS
176	174	95	101	95.2	39749	PASS
177	176	5	9	6.6	2628	PASS