

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061623\
 Data File : VU054565.D
 Acq On : 16 Jun 2023 11:45
 Operator : MD/SY
 Sample : 03253-11
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXYY4

Quant Time: Jun 17 06:13:16 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jun 17 06:10:25 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	258412	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	255667	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.808	152	125506	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.599	65	59889	3.642	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	72.800%
7) Chloroethane-d5	1.914	69	78648	5.108	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	102.200%
11) 1,1-Dichloroethene-d2	2.564	65	28202	3.840	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	76.800%
20) 2-Butanone-d5	4.628	46	244687	52.919	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	105.840%
24) Chloroform-d	5.059	84	175154	5.095	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.000%
26) 1,2-Dichloroethane-d4	5.698	65	87932	5.247	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.000%
32) Benzene-d6	5.724	84	333008	4.686	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.800%
36) 1,2-Dichloropropane-d6	6.686	67	120121	5.061	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.200%
41) Toluene-d8	7.895	98	271899	4.311	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.200%
43) trans-1,3-Dichloroprop...	8.177	79	34146	4.137	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	82.800%
46) 2-Hexanone-d5	8.628	63	166953	48.214	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.420%
56) 1,1,2,2-Tetrachloroeth...	10.750	84	89397	5.051	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	101.000%
66) 1,2-Dichlorobenzene-d4	12.187	152	108279	5.115	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.200%
Target Compounds						
					Qvalue	
13) Acetone	2.641	43	30849	7.076	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061623\
Data File : VU054565.D
Acq On : 16 Jun 2023 11:45
Operator : MD/SY
Sample : 03253-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXYY4

Quant Time: Jun 17 06:13:16 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jun 17 06:10:25 2023
Response via : Initial Calibration

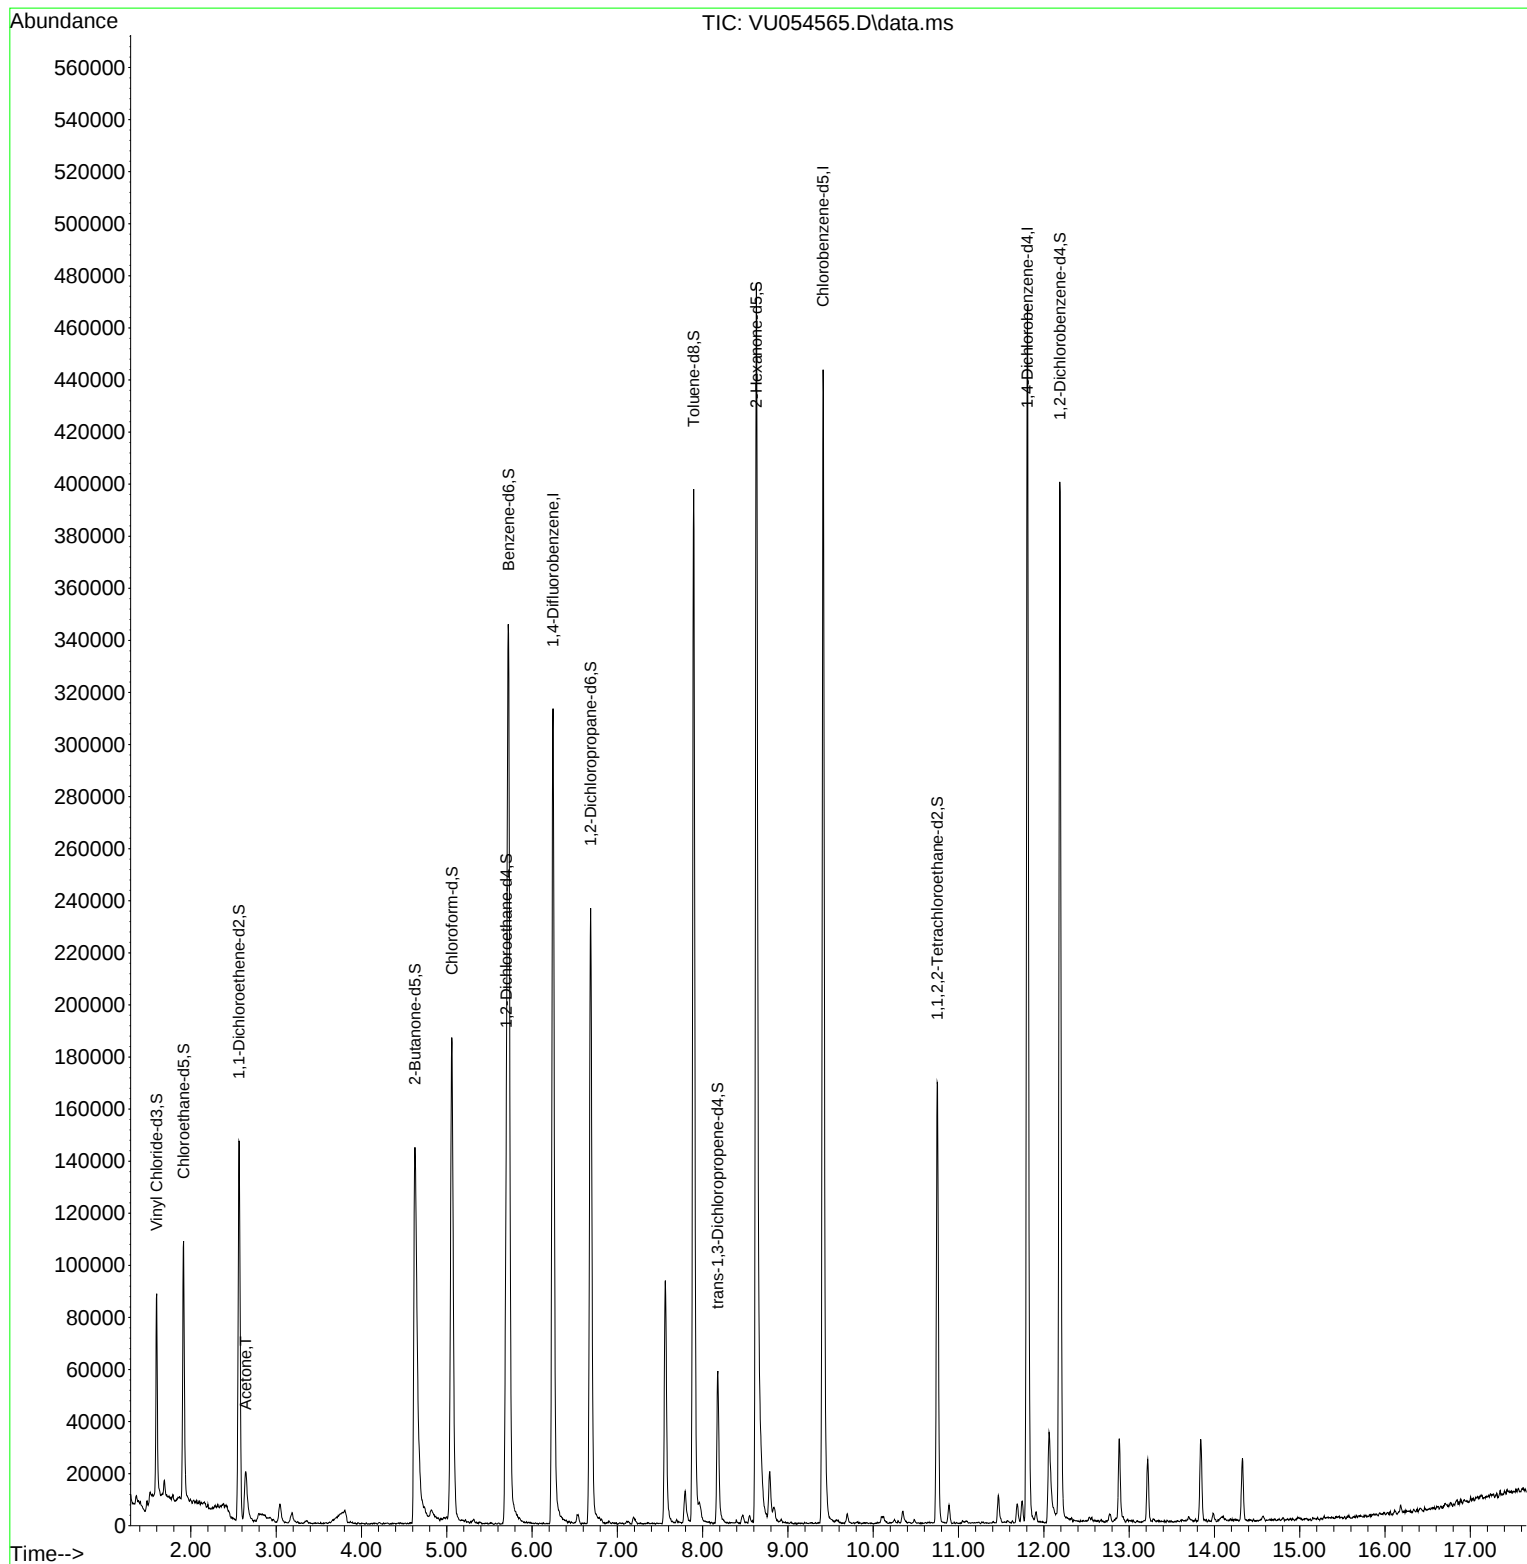

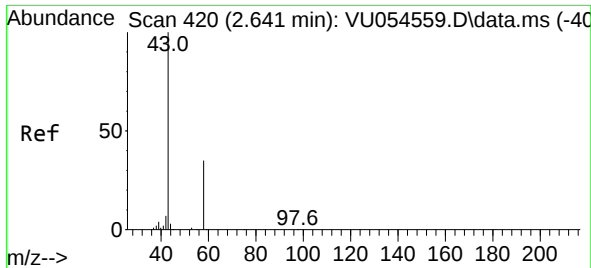

#13
 Acetone
 Concen: 7.076 ug/L
 RT: 2.641 min Scan# 41
 Delta R.T. 0.000 min
 Lab File: VU054565.D
 Acq: 16 Jun 2023 11:45

Instrument :
 MSVOA_U
 ClientSampleId :
 EXYY4

Tgt Ion: 43 Resp: 30849
 Ion Ratio Lower Upper
 43 100
 58 29.4 0.0 67.2

