

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061623\
 Data File : VU054560.D
 Acq On : 16 Jun 2023 09:38
 Operator : MD/SY
 Sample : VU0616WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK004

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU054560.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	89	96	110	rVB	80122	95742	10.78%	1.312%
2	1.914	185	194	211	rVB	98687	136875	15.41%	1.875%
3	2.567	385	397	414	rBV	138235	232687	26.20%	3.188%
4	4.631	1024	1039	1077	rBV2	130823	385795	43.44%	5.285%
5	5.058	1155	1172	1197	rVB	176148	395632	44.55%	5.420%
6	5.721	1358	1378	1410	rBV2	332248	878083	98.88%	12.029%
7	6.245	1528	1541	1570	rBV	304946	605021	68.13%	8.288%
8	6.534	1620	1631	1647	rVB	4437	9820	1.11%	0.135%
9	6.685	1665	1678	1696	rBV	219151	439173	49.46%	6.016%
10	7.563	1938	1951	1974	rBV2	85822	160177	18.04%	2.194%
11	7.894	2038	2054	2074	rBV	371702	658778	74.19%	9.024%
12	8.177	2130	2142	2161	rBV	53052	95246	10.73%	1.305%
13	8.631	2270	2283	2317	rBV2	440703	888016	100.00%	12.165%
14	9.415	2512	2527	2558	rBV	432454	743833	83.76%	10.190%
15	10.753	2930	2943	2962	rBV	161137	264867	29.83%	3.628%
16	11.807	3260	3271	3293	rBV	422571	692377	77.97%	9.485%
17	12.190	3377	3390	3410	rBV	346153	584320	65.80%	8.004%
18	13.839	3896	3903	3916	rBV4	6791	11274	1.27%	0.154%
19	14.093	3975	3982	3993	rBV3	5395	9272	1.04%	0.127%
20	14.331	4047	4056	4067	rBV4	8556	12907	1.45%	0.177%




Sum of corrected areas: 7299895

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061623\
Data File : VU054560.D
Acq On : 16 Jun 2023 09:38
Operator : MD/SY
Sample : VU0616WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK004

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

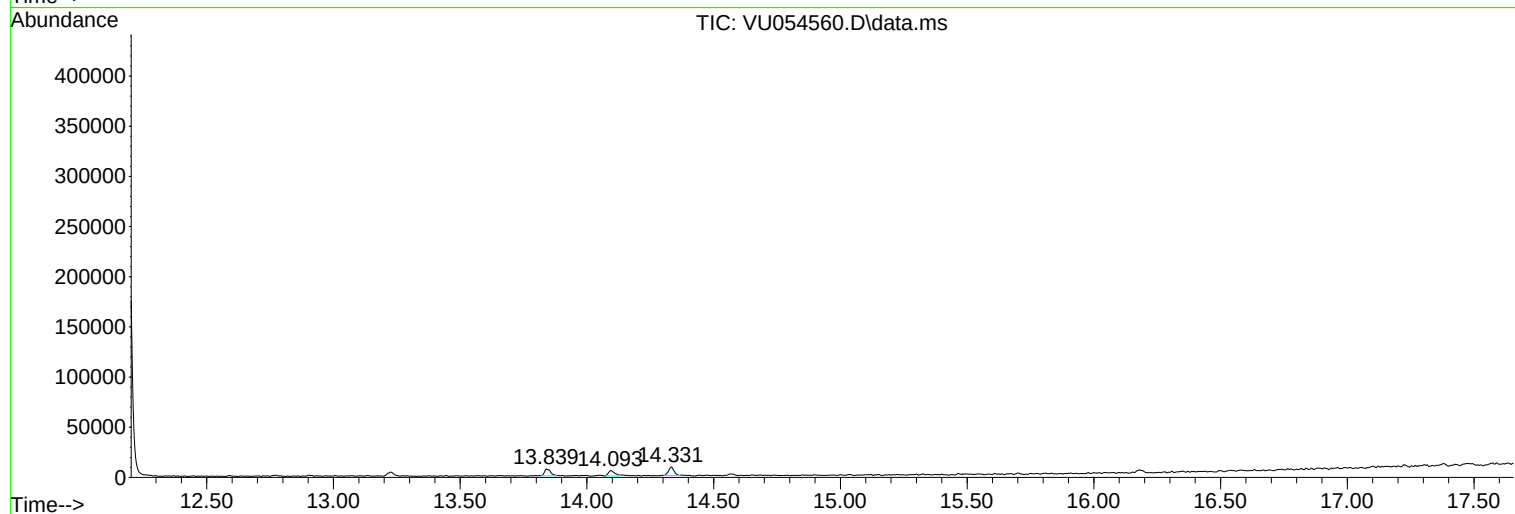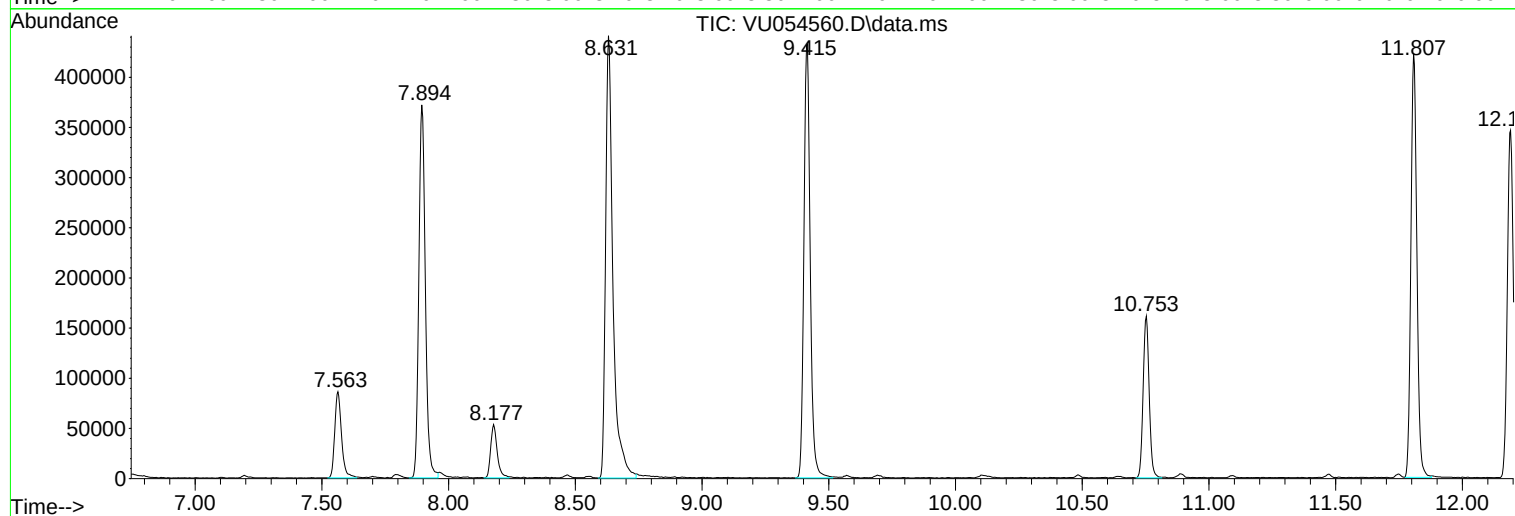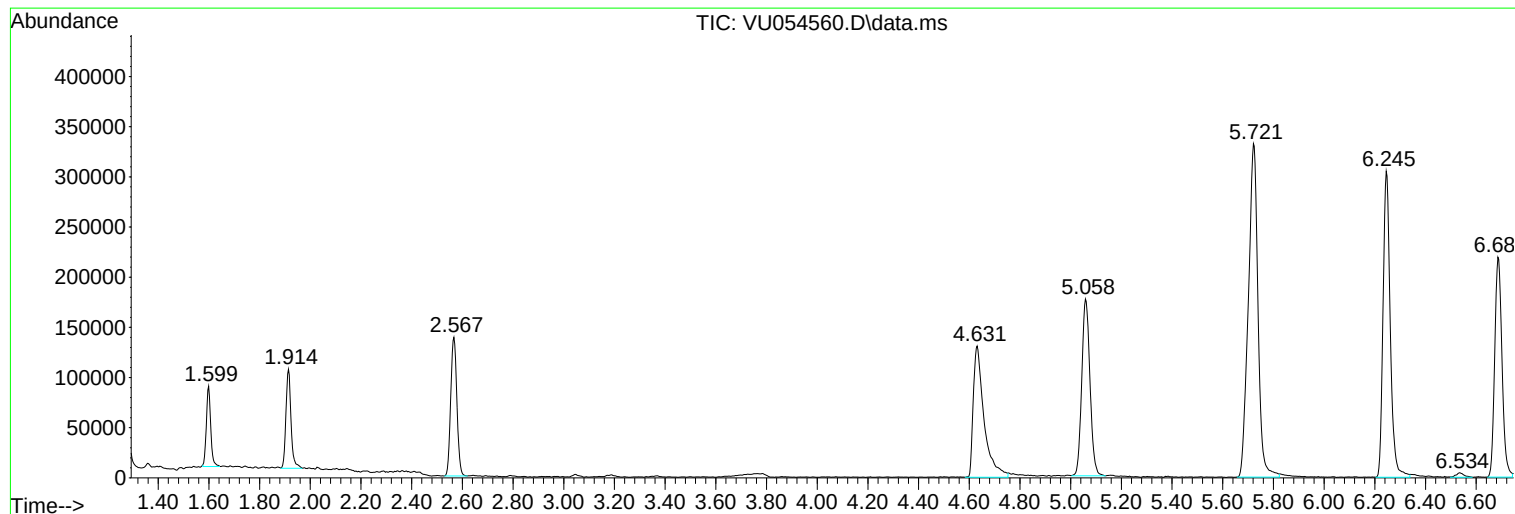

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061623\
Data File : VU054560.D
Acq On : 16 Jun 2023 09:38
Operator : MD/SY
Sample : VU0616WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK004

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061623\
Data File : VU054560.D
Acq On : 16 Jun 2023 09:38
Operator : MD/SY
Sample : VU0616WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK004

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc