

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061623\
 Data File : VU054562.D
 Acq On : 16 Jun 2023 10:33
 Operator : MD/SY
 Sample : 03253-03DL 5X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXYY0DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU054562.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	87	96	109	rBV2	98856	124058	11.37%	1.383%
2	1.914	186	194	207	rVB	98023	133748	12.25%	1.491%
3	2.566	385	397	414	rBV2	146574	247594	22.68%	2.760%
4	3.184	579	589	606	rVB2	8579	19345	1.77%	0.216%
5	3.865	784	801	827	rBV	107773	264197	24.20%	2.945%
6	4.660	1024	1048	1076	rBV2	337484	1091578	100.00%	12.167%
7	5.058	1157	1172	1197	rVB	177076	393851	36.08%	4.390%
8	5.316	1235	1252	1267	rBV3	60503	135743	12.44%	1.513%
9	5.721	1358	1378	1413	rBV2	335538	896485	82.13%	9.993%
10	6.245	1525	1541	1569	rBV	333122	659780	60.44%	7.354%
11	6.685	1663	1678	1697	rBV2	220688	442975	40.58%	4.938%
12	7.563	1938	1951	1976	rBV2	91090	168229	15.41%	1.875%
13	7.894	2041	2054	2071	rBV	373079	668354	61.23%	7.450%
14	7.965	2073	2076	2090	rVB3	9225	15491	1.42%	0.173%
15	8.177	2131	2142	2164	rBV	53482	98429	9.02%	1.097%
16	8.553	2250	2259	2267	rVB4	8789	14080	1.29%	0.157%
17	8.631	2271	2283	2321	rBV2	440453	926546	84.88%	10.328%
18	9.415	2511	2527	2555	rBV	453369	804253	73.68%	8.965%
19	9.569	2566	2575	2591	rVB2	7332	13226	1.21%	0.147%
20	9.698	2602	2615	2630	rVB2	14832	25557	2.34%	0.285%
21	10.116	2733	2745	2757	rBV6	8610	19439	1.78%	0.217%
22	10.753	2930	2943	2963	rBV	158376	261744	23.98%	2.918%
23	11.807	3259	3271	3293	rBV	465695	774276	70.93%	8.631%
24	12.190	3374	3390	3413	rBV	379780	656894	60.18%	7.322%
25	13.219	3701	3710	3727	rVB2	16609	29420	2.70%	0.328%
26	14.328	4043	4055	4068	rBV	51988	86068	7.88%	0.959%




Sum of corrected areas: 8971360

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061623\
Data File : VU054562.D
Acq On : 16 Jun 2023 10:33
Operator : MD/SY
Sample : 03253-03DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXYY0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

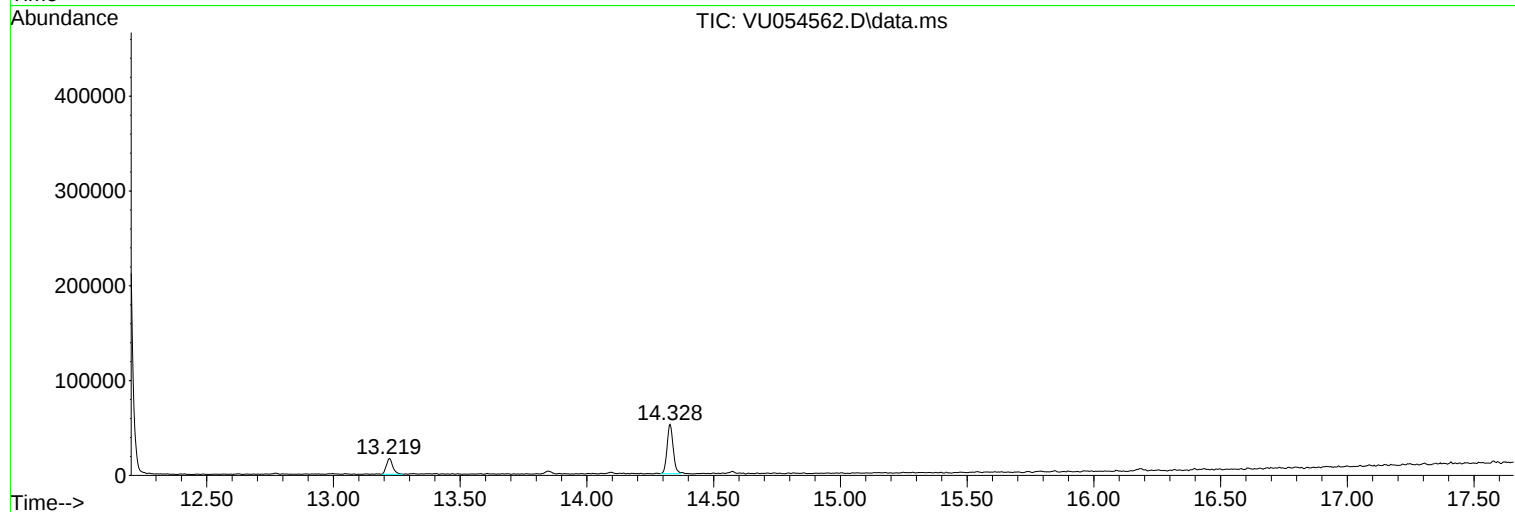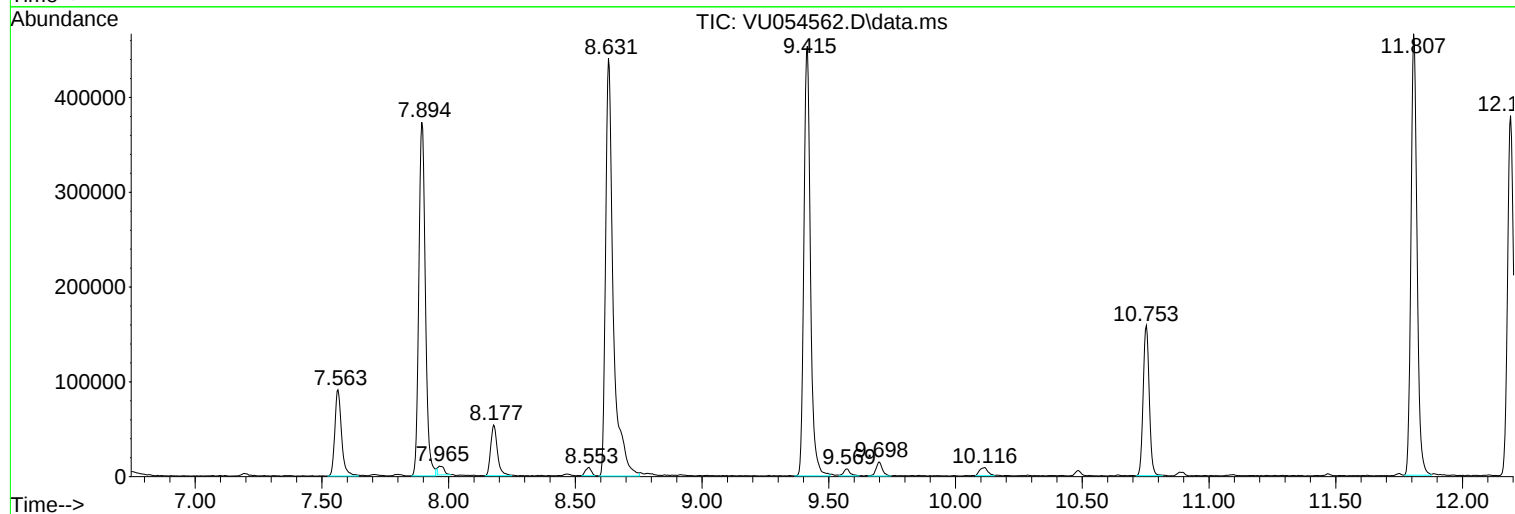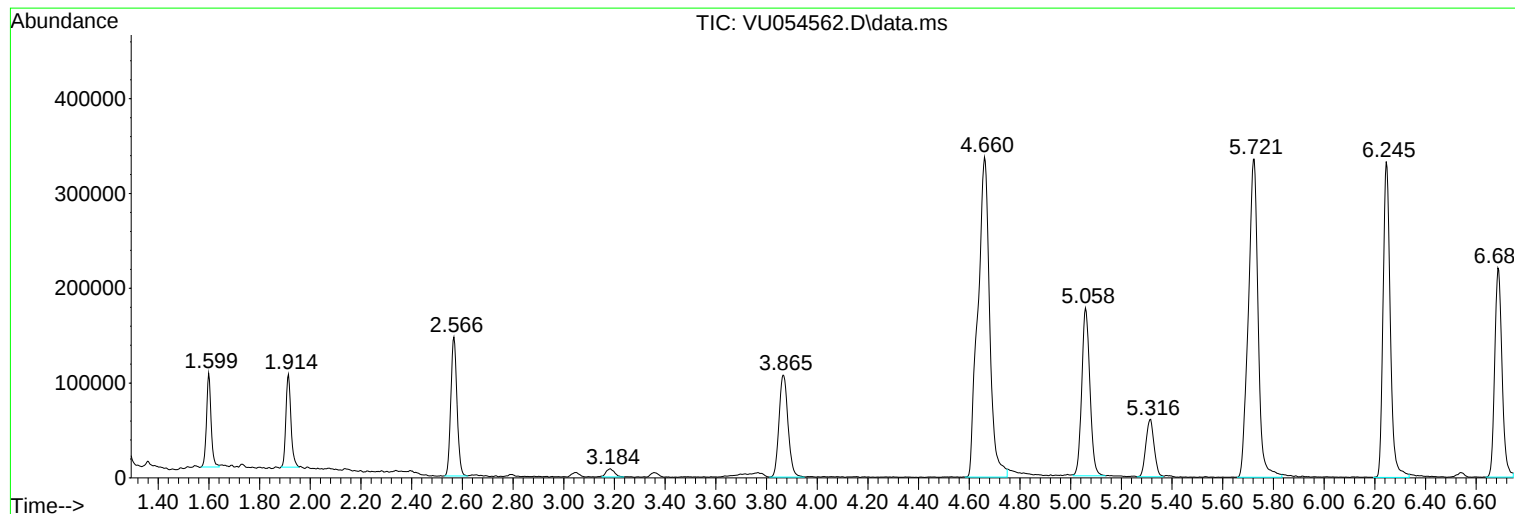

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061623\
Data File : VU054562.D
Acq On : 16 Jun 2023 10:33
Operator : MD/SY
Sample : 03253-03DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXYY0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061623\
Data File : VU054562.D
Acq On : 16 Jun 2023 10:33
Operator : MD/SY
Sample : 03253-03DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXYY0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------