

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061623\
 Data File : VU054567.D
 Acq On : 16 Jun 2023 12:33
 Operator : MD/SY
 Sample : 03284-04
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCGZ1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU054567.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	88	96	108	rVB	77228	91776	9.92%	1.231%
2	1.689	117	124	137	rBV	32636	46500	5.03%	0.624%
3	1.914	185	194	211	rBV	95004	135024	14.60%	1.811%
4	2.566	384	397	412	rBV	139906	230996	24.97%	3.098%
5	2.647	412	422	433	rVB3	6339	13686	1.48%	0.184%
6	4.631	1027	1039	1081	rBV	134125	394364	42.63%	5.289%
7	5.058	1157	1172	1193	rBV	174818	391576	42.33%	5.251%
8	5.721	1358	1378	1409	rBV2	333908	886161	95.80%	11.884%
9	6.245	1524	1541	1566	rBV	298171	589547	63.73%	7.906%
10	6.688	1663	1679	1698	rBV	220358	446147	48.23%	5.983%
11	7.563	1934	1951	1976	rBV2	90364	166408	17.99%	2.232%
12	7.894	2039	2054	2073	rBV	368530	664285	71.81%	8.908%
13	8.177	2132	2142	2160	rBV	53727	95148	10.29%	1.276%
14	8.630	2268	2283	2313	rBV2	458244	925000	100.00%	12.404%
15	8.791	2323	2333	2346	rVB8	11221	20662	2.23%	0.277%
16	9.415	2514	2527	2553	rBV	420012	720681	77.91%	9.664%
17	10.753	2929	2943	2963	rBV	163084	269045	29.09%	3.608%
18	10.888	2975	2985	3000	rVB2	9050	16176	1.75%	0.217%
19	11.807	3259	3271	3291	rBV	434035	704871	76.20%	9.452%
20	12.071	3341	3353	3369	rBV6	11466	29234	3.16%	0.392%
21	12.190	3375	3390	3409	rBV	373456	619723	67.00%	8.311%




Sum of corrected areas: 7457010

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061623\
Data File : VU054567.D
Acq On : 16 Jun 2023 12:33
Operator : MD/SY
Sample : 03284-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCGZ1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

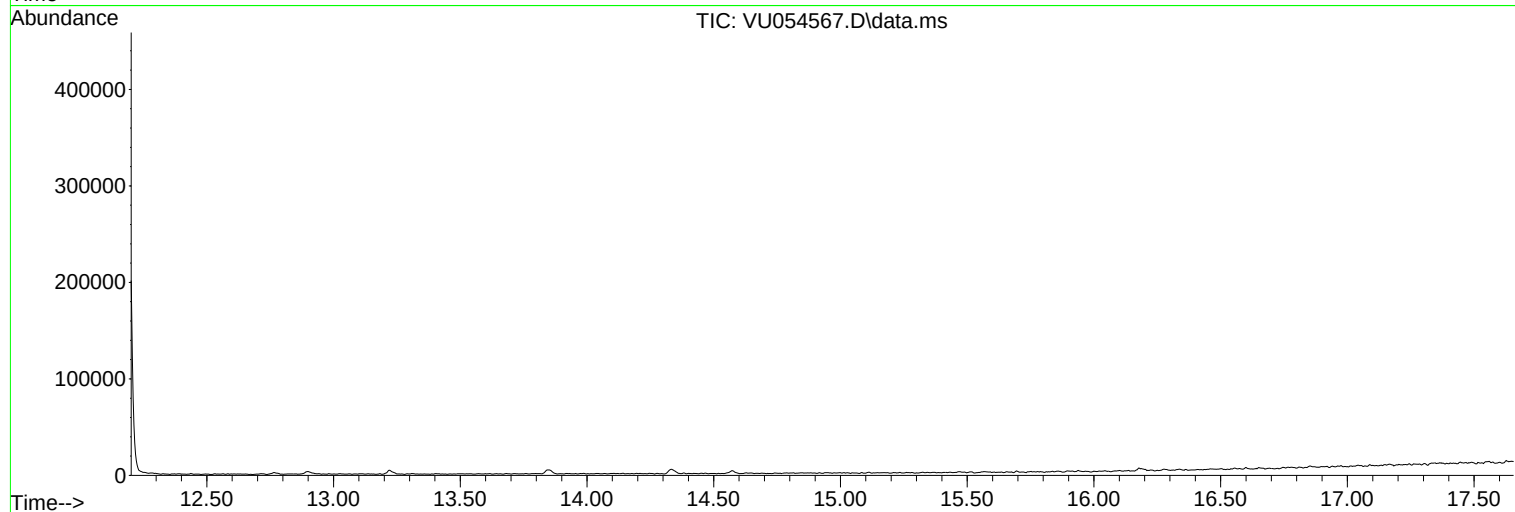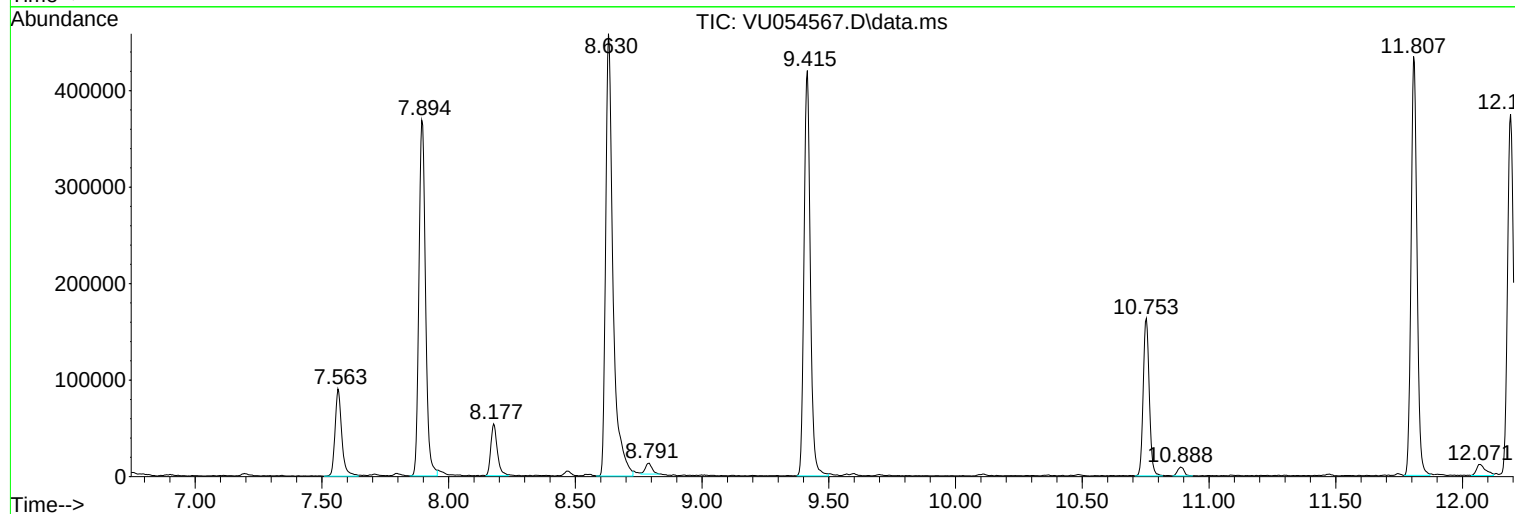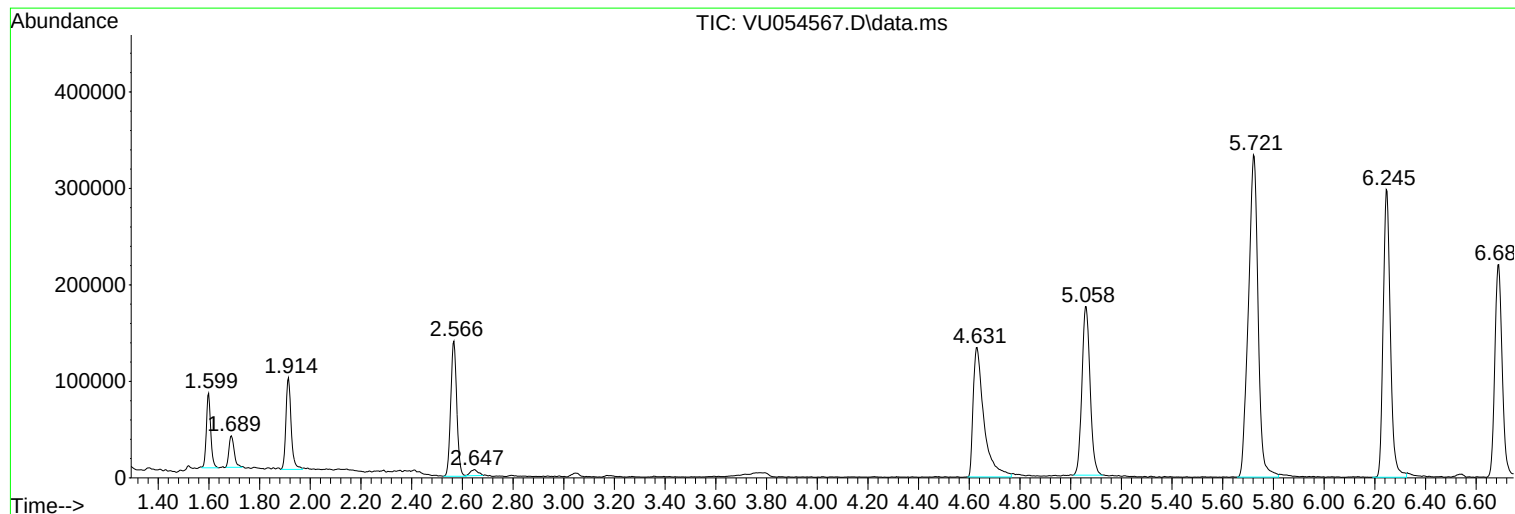

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061623\
Data File : VU054567.D
Acq On : 16 Jun 2023 12:33
Operator : MD/SY
Sample : 03284-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCGZ1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061623\
Data File : VU054567.D
Acq On : 16 Jun 2023 12:33
Operator : MD/SY
Sample : 03284-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCGZ1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc