

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061623\
 Data File : VU054571.D
 Acq On : 16 Jun 2023 14:10
 Operator : MD/SY
 Sample : 03284-06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCGZ3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU054571.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.306	3	5	15	rVB	27996	26220	2.59%	0.320%
2	1.357	18	21	34	rVB3	16017	19234	1.90%	0.235%
3	1.515	65	70	79	rBV3	7773	10503	1.04%	0.128%
4	1.599	87	96	112	rVB	80493	100899	9.95%	1.230%
5	1.730	132	137	148	rVB	21415	27227	2.68%	0.332%
6	1.914	186	194	212	rVB	100483	141128	13.91%	1.721%
7	2.566	385	397	411	rBV	142192	235273	23.20%	2.869%
8	2.640	413	420	438	rVB	9162	20007	1.97%	0.244%
9	3.187	577	590	601	rBV2	8180	19969	1.97%	0.244%
10	3.357	632	643	654	rVB4	6610	13662	1.35%	0.167%
11	3.865	784	801	817	rBV2	17107	41063	4.05%	0.501%
12	4.627	1026	1038	1079	rBV3	158598	612879	60.42%	7.474%
13	5.062	1153	1173	1193	rBV2	184041	418756	41.29%	5.106%
14	5.721	1358	1378	1407	rBV2	352587	951146	93.77%	11.598%
15	6.245	1529	1541	1564	rBV	299232	587145	57.89%	7.160%
16	6.541	1622	1633	1647	rVB7	18851	36330	3.58%	0.443%
17	6.688	1665	1679	1697	rBV	237219	472649	46.60%	5.764%
18	7.563	1939	1951	1980	rBV2	94696	176409	17.39%	2.151%
19	7.894	2038	2054	2087	rBV	382484	703279	69.34%	8.576%
20	8.177	2132	2142	2164	rBV	57695	104063	10.26%	1.269%
21	8.470	2220	2233	2246	rBV2	7259	13029	1.28%	0.159%
22	8.630	2270	2283	2320	rBV2	502044	1014290	100.00%	12.368%
23	8.788	2325	2332	2346	rVB7	6938	12796	1.26%	0.156%
24	9.415	2514	2527	2553	rBV	417818	727374	71.71%	8.870%
25	9.598	2571	2584	2596	rVB4	5558	10874	1.07%	0.133%
26	10.753	2927	2943	2957	rBV	177327	290277	28.62%	3.540%
27	10.891	2976	2986	2995	rVB2	14262	22215	2.19%	0.271%
28	11.807	3259	3271	3298	rBV	430043	714401	70.43%	8.712%
29	12.068	3345	3352	3359	rBV8	5911	11850	1.17%	0.145%
30	12.190	3377	3390	3410	rBV	400187	665653	65.63%	8.117%




Sum of corrected areas: 8200600

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061623\
Data File : VU054571.D
Acq On : 16 Jun 2023 14:10
Operator : MD/SY
Sample : 03284-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCGZ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

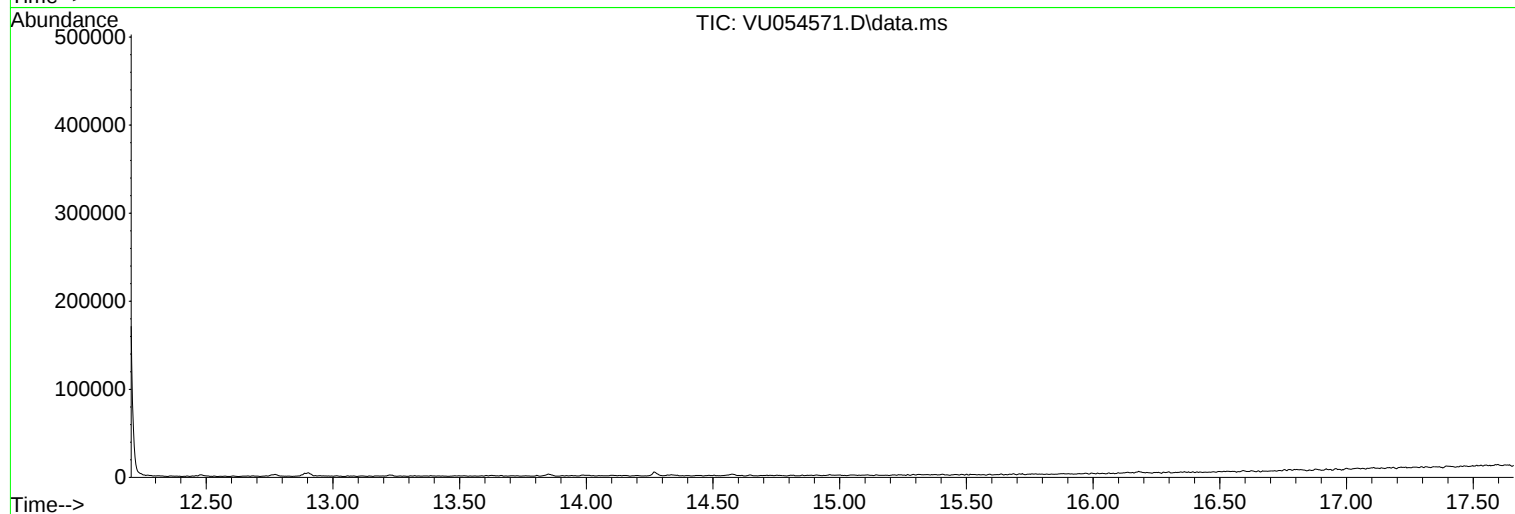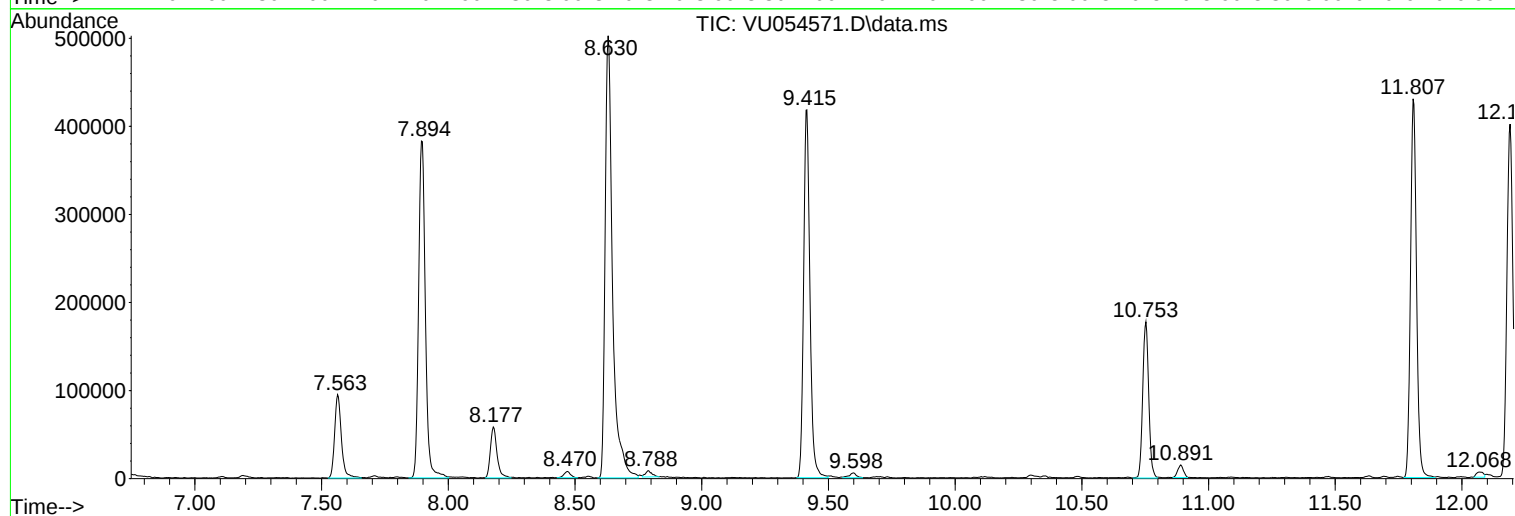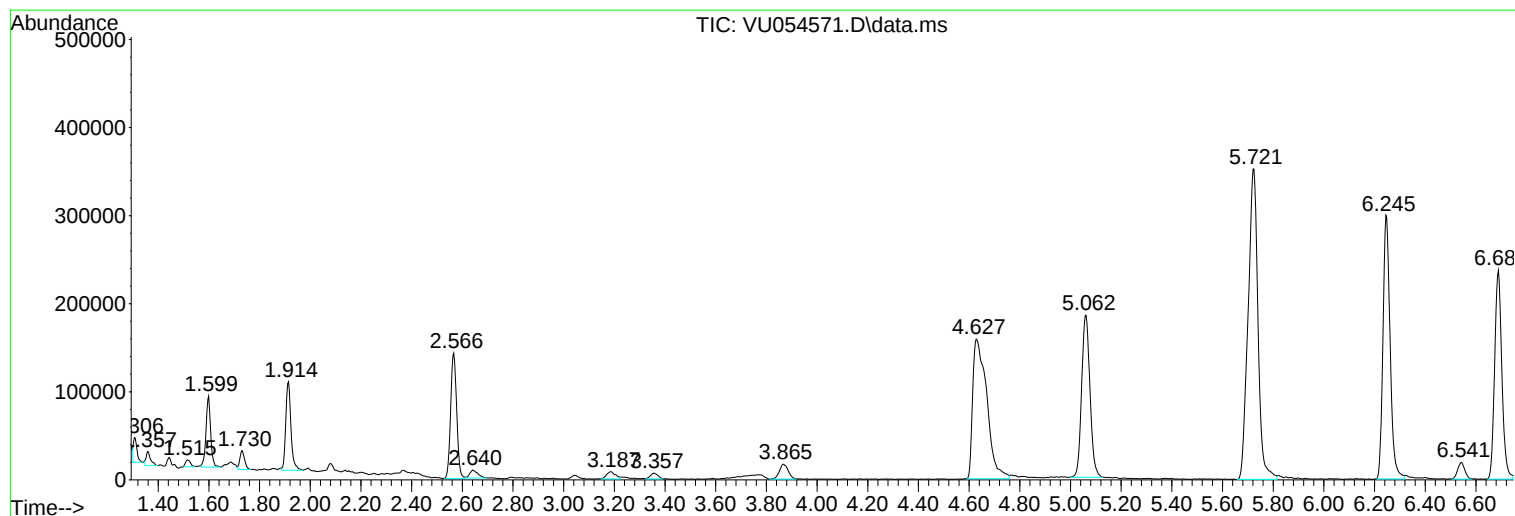

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061623\
Data File : VU054571.D
Acq On : 16 Jun 2023 14:10
Operator : MD/SY
Sample : 03284-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCGZ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061623\
Data File : VU054571.D
Acq On : 16 Jun 2023 14:10
Operator : MD/SY
Sample : 03284-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCGZ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------