

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061623\
 Data File : VU054575.D
 Acq On : 16 Jun 2023 15:46
 Operator : MD/SY
 Sample : 03284-12
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCGZ7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU054575.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.361	17	22	41	rVB3	19451	27681	2.80%	0.355%
2	1.489	57	62	66	rBV	13054	11974	1.21%	0.154%
3	1.599	88	96	107	rBV	88913	105211	10.64%	1.349%
4	1.911	186	193	210	rVB	100062	136718	13.83%	1.753%
5	1.994	215	219	227	rVB2	11364	13743	1.39%	0.176%
6	2.200	278	283	295	rVB3	8913	12511	1.27%	0.160%
7	2.367	328	335	345	rVB4	11178	18267	1.85%	0.234%
8	2.567	384	397	412	rBV	140171	237330	24.01%	3.043%
9	2.637	412	419	435	rVB2	6328	13091	1.32%	0.168%
10	3.708	734	752	757	rBV6	4421	12405	1.25%	0.159%
11	3.866	788	801	817	rBV2	17921	43070	4.36%	0.552%
12	4.624	1024	1037	1075	rBV	154725	440872	44.60%	5.652%
13	5.058	1154	1172	1194	rVB	183782	410292	41.51%	5.260%
14	5.312	1238	1251	1264	rVB3	14189	31180	3.15%	0.400%
15	5.721	1358	1378	1408	rBV2	354119	922795	93.35%	11.831%
16	6.245	1528	1541	1566	rBV	286187	568808	57.54%	7.293%
17	6.541	1621	1633	1647	rVB7	8176	17513	1.77%	0.225%
18	6.685	1664	1678	1696	rBV	238154	467587	47.30%	5.995%
19	7.563	1939	1951	1966	rBV2	90042	167364	16.93%	2.146%
20	7.894	2041	2054	2073	rBV	383432	683438	69.14%	8.762%
21	8.177	2132	2142	2164	rBV2	55097	98197	9.93%	1.259%
22	8.631	2271	2283	2315	rBV2	496487	988531	100.00%	12.674%
23	9.415	2514	2527	2550	rBV	403968	706250	71.44%	9.055%
24	10.753	2930	2943	2959	rBV	176595	287134	29.05%	3.681%
25	10.891	2976	2986	2998	rVB	10139	16728	1.69%	0.214%
26	11.807	3260	3271	3293	rBV	423144	690010	69.80%	8.847%
27	12.068	3339	3352	3363	rBV6	9619	22562	2.28%	0.289%
28	12.190	3377	3390	3406	rBV	394453	648444	65.60%	8.314%




Sum of corrected areas: 7799706

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061623\
Data File : VU054575.D
Acq On : 16 Jun 2023 15:46
Operator : MD/SY
Sample : 03284-12
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCGZ7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

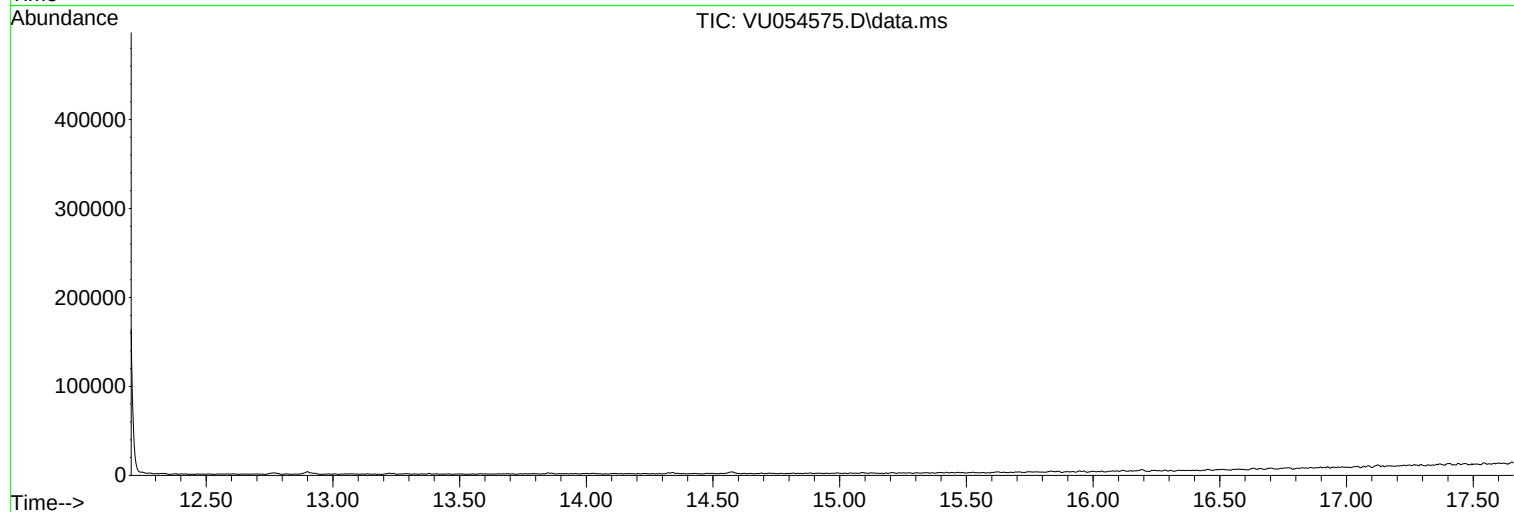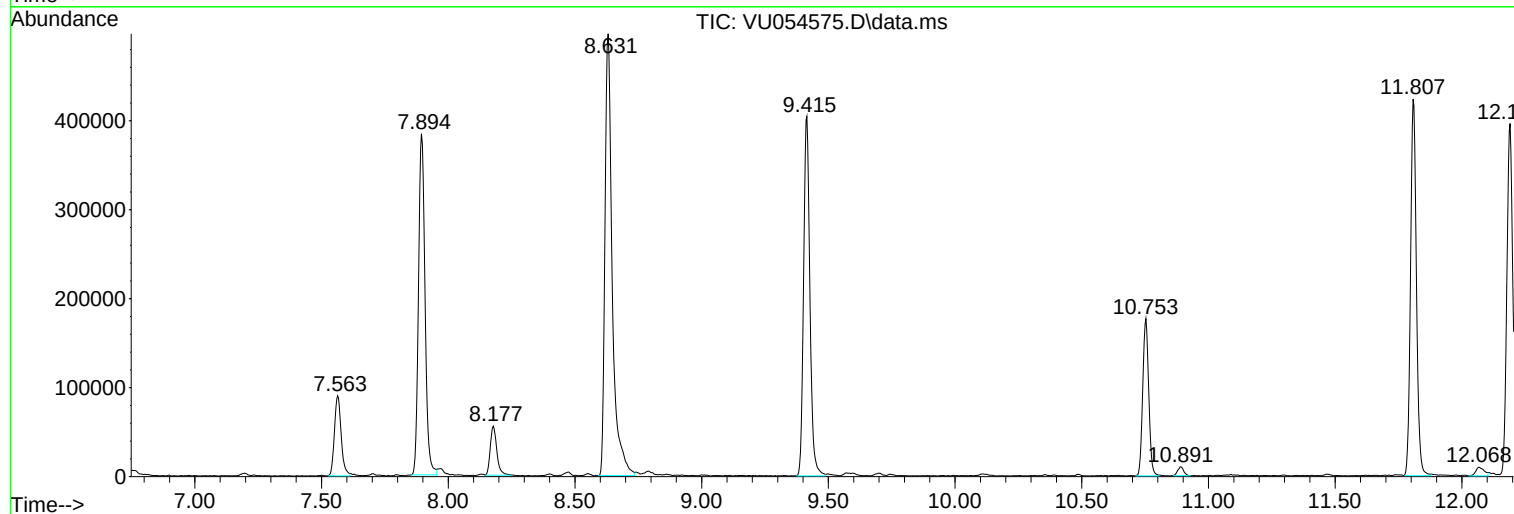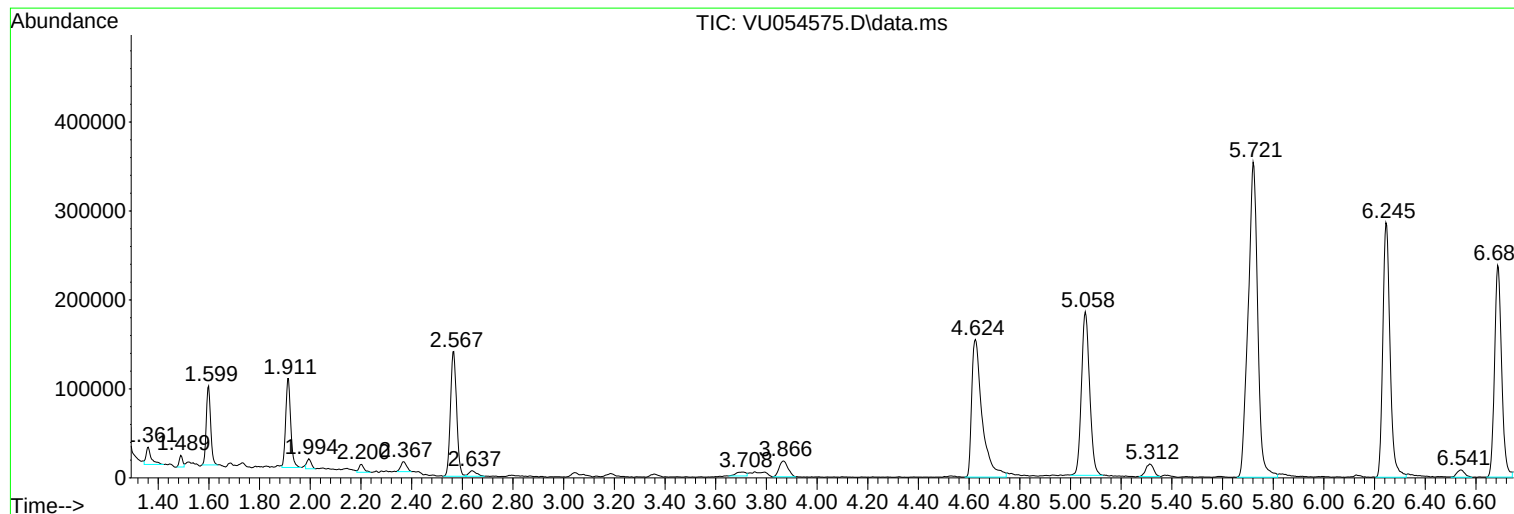

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061623\
Data File : VU054575.D
Acq On : 16 Jun 2023 15:46
Operator : MD/SY
Sample : 03284-12
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCGZ7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061623\
Data File : VU054575.D
Acq On : 16 Jun 2023 15:46
Operator : MD/SY
Sample : 03284-12
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCGZ7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc