
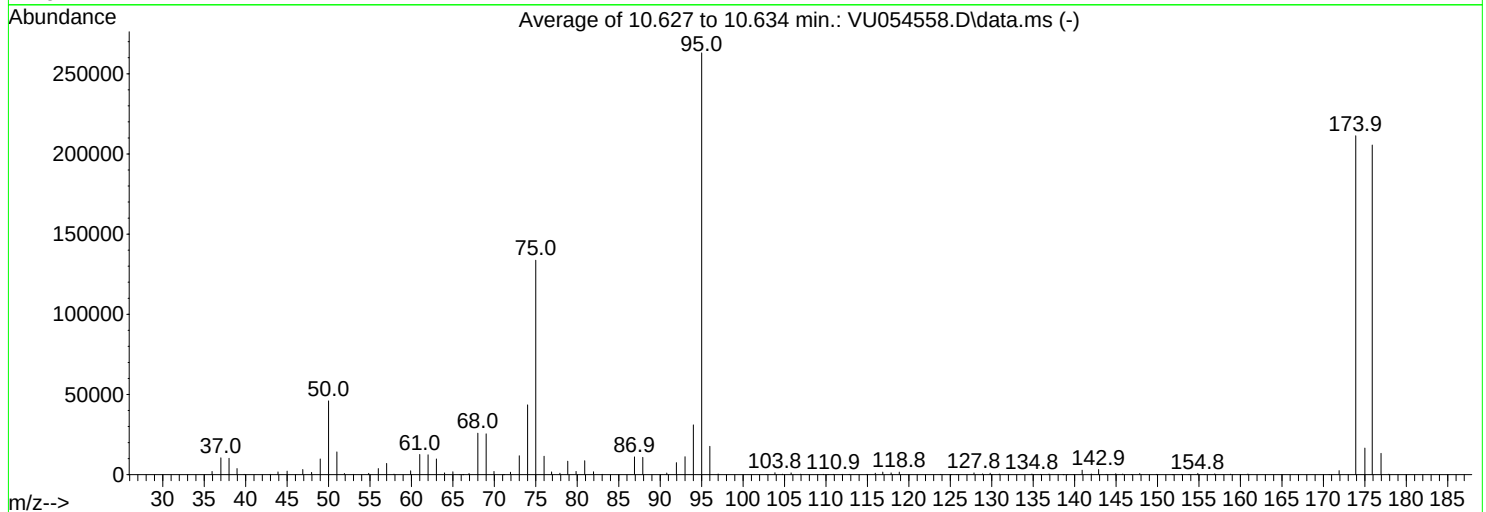


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061623\
Data File : VU054558.D
Acq On : 16 Jun 2023 08:19
Operator : MD/SY
Sample : BFB020
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB020

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sat Jun 17 06:10:25 2023

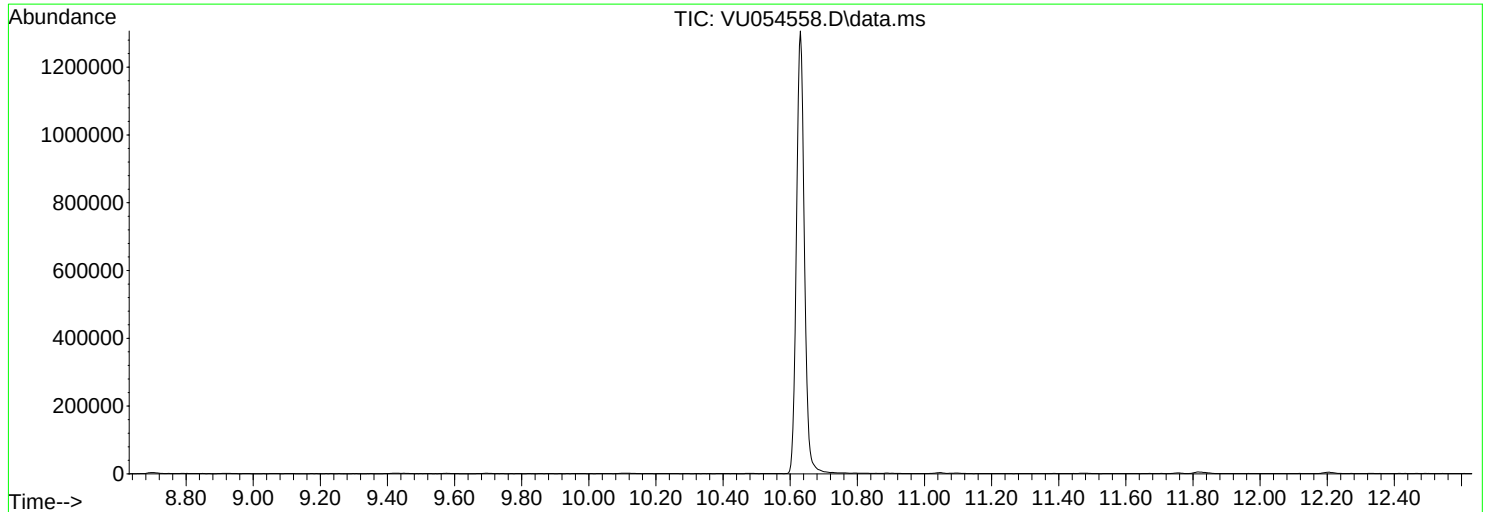

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.5	46040	PASS
75	95	30	80	50.8	133685	PASS
95	95	100	100	100.0	263061	PASS
96	95	5	9	6.7	17696	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	80.3	211349	PASS
175	174	5	9	7.8	16563	PASS
176	174	95	101	97.3	205547	PASS
177	176	5	9	6.5	13280	PASS

m/z	Abundance
39.70	212.0
44.00	440.0

Instrument :
MSVOA_U
ClientSampleId :
BFB020

m/z	Abundance
36.00	1897.0
37.00	10645.0
38.00	10104.0
38.90	3924.0
39.90	351.0
42.90	188.0
43.90	2168.0
45.00	2259.0
46.90	3079.0
48.00	1450.0
49.00	9806.0
50.00	47568.0
51.00	14581.0
51.90	715.0
53.00	205.0
54.90	759.0
56.00	3817.0
57.00	7030.0
57.90	301.0
59.90	2371.0
61.00	13124.0
62.00	12212.0
63.00	9762.0
64.00	1113.0
65.00	1754.0
65.80	248.0
66.90	634.0
68.00	25648.0
69.00	25200.0
70.00	1920.0
72.00	1484.0
73.00	12202.0
74.00	43928.0
75.00	135552.0
76.00	11867.0
76.90	1762.0
77.80	845.0
78.80	8696.0
79.90	2003.0
80.90	8537.0
81.90	1751.0
83.00	214.0
86.90	11195.0
87.90	10402.0
90.80	1155.0
91.90	7371.0
93.00	11148.0
94.00	31120.0
95.00	263488.0
96.00	18088.0
97.00	410.0
102.70	157.0
103.80	1222.0
104.70	327.0
105.80	1169.0
106.90	262.0
109.70	133.0
110.90	196.0
112.00	240.0
112.80	192.0
115.00	214.0
115.90	975.0
116.90	1635.0
117.80	1022.0
118.90	1723.0
123.90	186.0
127.90	1113.0
128.90	504.0
129.90	855.0
130.90	375.0
134.80	379.0
135.90	163.0
136.90	506.0
139.10	130.0
139.90	127.0
140.90	2805.0
142.10	480.0
142.90	3225.0
143.80	270.0
145.00	696.0
145.80	464.0
146.90	163.0
147.90	716.0
149.90	177.0
152.90	195.0
153.90	219.0
154.90	731.0
155.70	119.0
156.90	522.0
158.80	275.0
160.90	302.0
170.70	234.0

Instrument :
MSVOA_U
ClientSampleId :
BFB020

171.90	2224.0
173.90	206144.0
175.00	16752.0
175.90	201216.0
176.90	13171.0
177.90	318.0

Instrument :
MSVOA_U
ClientSampleId :
BFB020

m/z	Abundance
36.00	2099.0
37.00	10775.0
38.00	10446.0
39.00	3945.0
39.90	392.0
42.90	194.0
43.90	2284.0
45.00	2346.0
46.10	267.0
46.90	3260.0
48.00	1371.0
49.00	10066.0
50.00	47472.0
51.00	14409.0
51.90	777.0
53.00	213.0
54.80	798.0
56.00	3826.0
57.00	7199.0
57.90	264.0
59.90	2446.0
61.00	13099.0
62.00	12655.0
63.00	10044.0
64.00	1106.0
65.00	1871.0
65.90	151.0
67.00	664.0
68.00	26704.0
69.00	26160.0
69.90	2012.0
71.90	1489.0
73.00	12259.0
74.00	44872.0
75.00	137856.0
76.00	11877.0
76.90	1733.0
77.90	885.0
78.80	8632.0
79.80	2096.0
80.90	8933.0
82.00	1841.0
83.00	218.0
86.90	11549.0
87.90	11220.0
90.80	1033.0
92.00	7705.0
93.00	11580.0
94.00	31736.0
95.00	270464.0
96.00	18120.0
97.00	478.0
102.80	160.0
103.80	1256.0
104.80	339.0
105.80	1086.0
107.00	251.0
109.70	186.0
110.20	131.0
110.90	267.0
111.90	224.0
112.80	207.0
115.00	201.0
115.90	920.0
116.80	1622.0
117.90	1189.0
118.90	1681.0
123.80	197.0
125.80	141.0
127.80	1204.0
128.90	483.0
129.80	914.0
130.90	470.0
134.90	433.0
135.90	182.0
136.90	476.0
139.20	100.0
139.90	137.0
140.90	2946.0
142.00	459.0
142.90	3335.0
143.80	265.0
145.00	642.0
145.80	425.0
146.80	141.0
147.80	702.0
149.90	229.0
152.90	221.0
153.80	200.0
154.80	818.0
155.70	144.0
156.90	541.0

Instrument :
MSVOA_U
ClientSampleId :
BFB020

157.90	151.0
158.80	313.0
160.90	409.0
171.90	2614.0
173.90	217920.0
175.00	17032.0
175.90	212544.0
176.90	13817.0
177.90	366.0

Instrument :
MSVOA_U
ClientSampleId :
BFB020

m/z	Abundance
35.90	2070.0
37.00	9992.0
38.00	9899.0
39.00	3657.0
39.90	432.0
43.00	221.0
43.90	2120.0
45.00	2109.0
46.00	204.0
46.90	3226.0
47.90	1423.0
49.00	9523.0
50.00	43080.0
51.00	13584.0
51.90	715.0
53.00	186.0
54.80	777.0
56.00	3669.0
57.00	6778.0
57.90	266.0
59.90	2315.0
61.00	11636.0
62.00	12172.0
63.00	9440.0
64.00	992.0
65.00	1683.0
66.20	176.0
67.00	699.0
68.00	25208.0
69.00	24864.0
69.90	1934.0
71.10	102.0
71.90	1482.0
73.00	10980.0
74.00	41648.0
75.00	127648.0
76.00	10849.0
76.90	1504.0
78.00	936.0
78.90	7803.0
79.80	1913.0
80.90	8494.0
81.90	1717.0
83.00	200.0
86.90	10615.0
87.90	10811.0
90.80	900.0
92.00	7560.0
93.00	10837.0
94.00	30152.0
95.00	255232.0
96.00	16880.0
97.00	500.0
102.90	149.0
103.90	1197.0
104.80	307.0
105.80	919.0
106.90	285.0
109.70	200.0
110.30	111.0
110.90	281.0
111.90	178.0
112.80	190.0
114.80	200.0
116.00	814.0
116.80	1518.0
117.90	1166.0
118.80	1440.0
123.70	228.0
125.00	113.0
125.80	151.0
127.90	1066.0
128.90	421.0
129.70	883.0
130.90	493.0
134.90	521.0
135.90	137.0
136.90	391.0
138.60	154.0
139.90	123.0
140.90	2752.0
141.90	414.0
142.90	3142.0
143.80	223.0
144.90	565.0
145.80	338.0
146.80	132.0
147.80	655.0
149.80	296.0
151.80	121.0
152.90	196.0
153.70	146.0

Instrument :
MSVOA_U
ClientSampleId :
BFB020

154.80	778.0
155.70	114.0
156.90	509.0
157.90	171.0
158.80	351.0
160.90	430.0
171.90	2515.0
173.90	209984.0
175.00	15906.0
175.90	202880.0
177.00	12853.0
177.90	350.0

Instrument :
MSVOA_U
ClientSampleId :
BFB020