
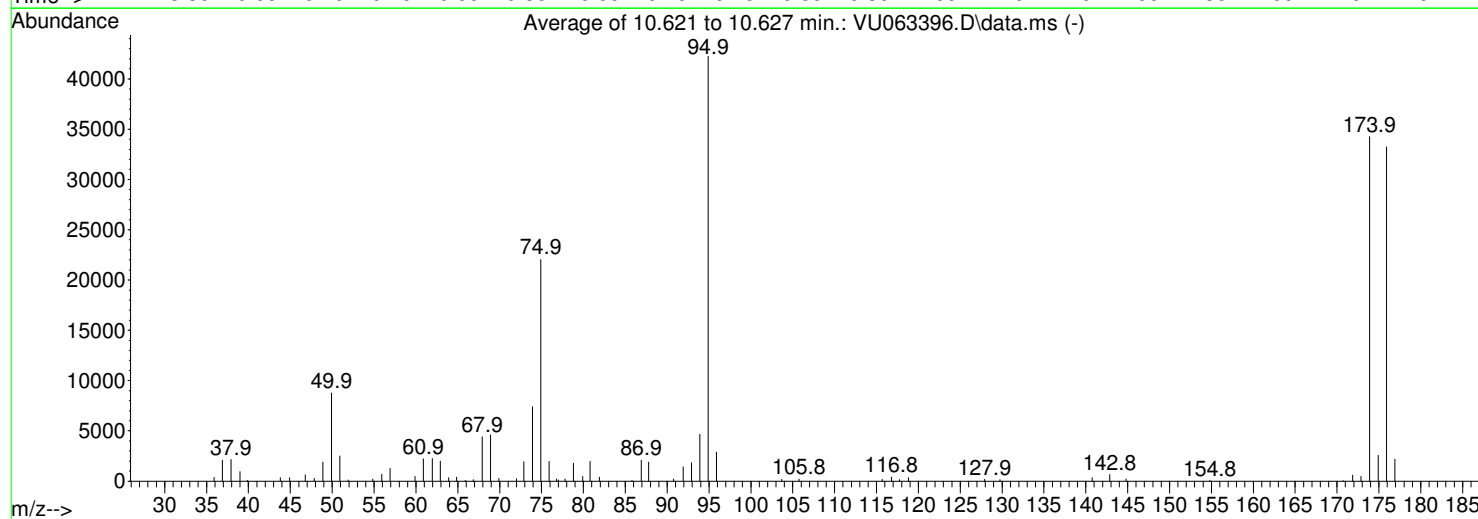


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061625\
Data File : VU063396.D
Acq On : 16 Jun 2025 09:01
Operator : MD/SY
Sample : BFB024
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB024

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM061625.M
Title : TRACE VOA SOM01.0
Last Update : Mon Jun 16 13:24:10 2025

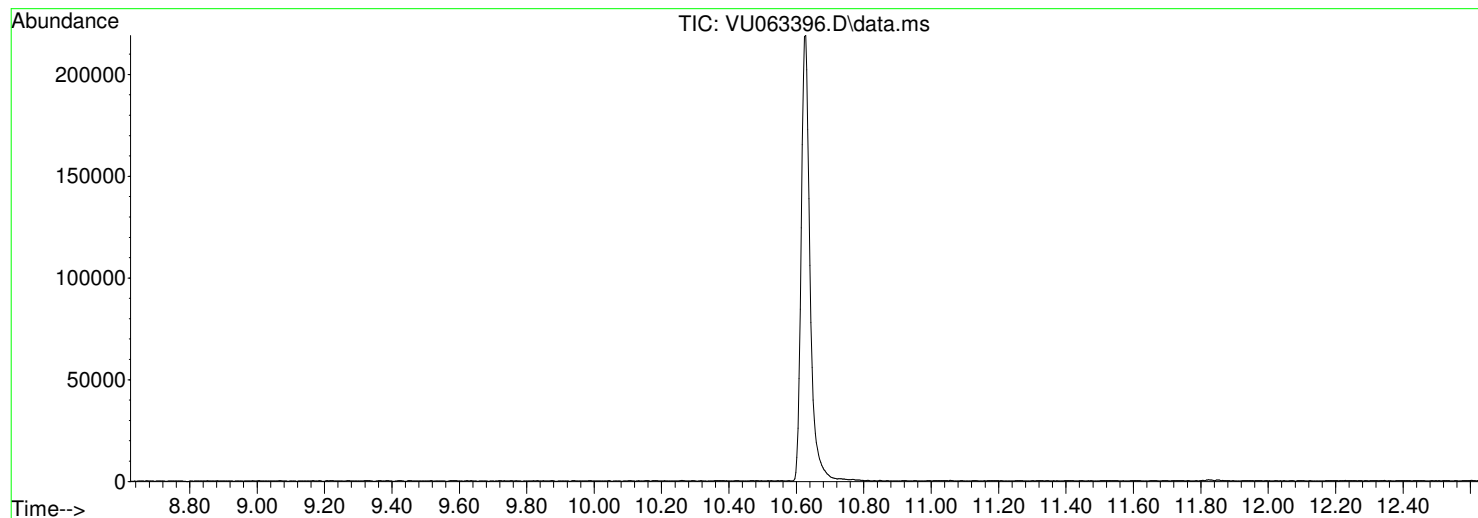

AutoFind: Scans 2902, 2903, 2904; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.7	8754	PASS
75	95	30	80	52.2	22056	PASS
95	95	100	100	100.0	42253	PASS
96	95	5	9	6.8	2866	PASS
173	174	0.00	2	1.3	462	PASS
174	95	50	120	81.1	34272	PASS
175	174	5	9	7.5	2564	PASS
176	174	95	101	97.0	33235	PASS
177	176	5	9	6.6	2180	PASS

m/z	Abundance
43.80	238.0

Instrument :
MSVOA_U
ClientSampleId :
BFB024

m/z	Abundance
35.90	339.0
36.90	2038.0
37.90	1937.0
39.00	933.0
43.80	533.0
44.90	322.0
46.80	638.0
47.90	243.0
48.90	1863.0
49.90	8186.0
50.90	2336.0
51.90	115.0
54.80	168.0
55.90	629.0
56.90	1121.0
59.90	446.0
60.90	2109.0
62.00	2137.0
62.90	1879.0
63.90	346.0
64.80	337.0
66.80	142.0
67.90	4150.0
68.90	4349.0
69.90	265.0
72.00	239.0
72.90	1706.0
73.90	7045.0
74.90	21136.0
75.90	1833.0
76.80	318.0
77.80	230.0
78.80	1749.0
79.90	471.0
80.80	1871.0
81.90	361.0
85.80	113.0
86.90	1984.0
87.80	1827.0
90.80	200.0
91.90	1255.0
92.90	1708.0
93.90	4390.0
94.90	39904.0
95.90	2776.0
103.70	172.0
105.70	187.0
115.70	149.0
116.80	332.0
117.80	119.0
118.80	332.0
127.90	141.0
129.80	114.0
140.70	315.0
142.90	569.0
144.90	185.0
171.80	559.0
172.90	447.0
173.90	31920.0
174.90	2396.0
175.90	30464.0
176.90	2028.0

Instrument :
MSVOA_U
ClientSampleId :
BFB024

m/z	Abundance
35.90	383.0
36.90	2154.0
37.90	2202.0
39.00	996.0
39.80	118.0
43.80	585.0
44.90	352.0
46.80	626.0
47.80	270.0
48.90	1951.0
49.90	9086.0
50.90	2585.0
51.90	143.0
54.90	221.0
55.90	690.0
56.90	1285.0
59.90	469.0
60.90	2246.0
62.00	2310.0
62.90	2036.0
63.90	352.0
64.80	398.0
65.90	108.0
66.80	152.0
67.90	4526.0
68.90	4763.0
69.90	271.0
72.00	233.0
72.90	1952.0
73.90	7521.0
74.90	22640.0
75.90	2033.0
76.80	334.0
77.80	216.0
78.80	1826.0
79.90	472.0
80.80	2045.0
81.90	403.0
85.80	117.0
86.90	2136.0
87.80	1955.0
90.70	206.0
91.90	1490.0
92.90	1867.0
93.90	4750.0
94.90	43488.0
95.90	2992.0
103.70	185.0
105.70	229.0
115.70	177.0
116.80	423.0
117.70	144.0
118.80	362.0
127.90	183.0
129.80	131.0
140.70	354.0
142.90	660.0
144.80	198.0
154.80	119.0
170.70	108.0
171.90	610.0
172.80	469.0
173.90	35176.0
174.90	2621.0
175.90	34248.0
176.90	2261.0

Instrument :
MSVOA_U
ClientSampleId :
BFB024

m/z	Abundance
35.90	401.0
36.90	2066.0
37.90	2299.0
39.00	903.0
39.90	156.0
43.90	593.0
44.90	344.0
46.80	575.0
47.80	275.0
48.90	1874.0
49.90	8991.0
50.90	2589.0
51.90	130.0
54.90	218.0
55.90	721.0
56.90	1378.0
59.90	464.0
60.90	2238.0
61.90	2330.0
62.90	2091.0
63.90	337.0
64.90	427.0
65.90	122.0
66.90	132.0
67.90	4509.0
68.90	4691.0
69.90	269.0
72.00	223.0
72.90	2081.0
73.90	7612.0
74.90	22392.0
75.90	2023.0
77.00	324.0
77.80	201.0
78.80	1759.0
79.90	479.0
80.80	1945.0
81.90	407.0
86.90	2091.0
87.80	1923.0
90.70	194.0
91.90	1526.0
92.90	1897.0
93.90	4832.0
94.90	43368.0
95.90	2831.0
103.70	161.0
105.80	231.0
115.70	173.0
116.80	423.0
117.70	152.0
118.80	350.0
127.90	198.0
129.70	146.0
140.80	376.0
142.80	698.0
144.70	203.0
154.80	144.0
171.90	605.0
172.80	471.0
173.90	35720.0
174.90	2674.0
175.90	34992.0
176.90	2251.0

Instrument :
MSVOA_U
ClientSampleId :
BFB024