

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU061719\
Quantitation Report (QT/LSC Reviewed)


Data File : VU032788.D
Acq On : 17 Jun 2019 17:27
Operator : JC/SP
Sample : K3363-07ME
Misc : 3.26g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0JX0ME

Manual Integrations
APPROVED

MMDadoda
6/18/2019 11:28:01 AM

Quant Time: Jun 18 04:19:58 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM061719WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 18 02:39:23 2019
Response via : Initial Calibration

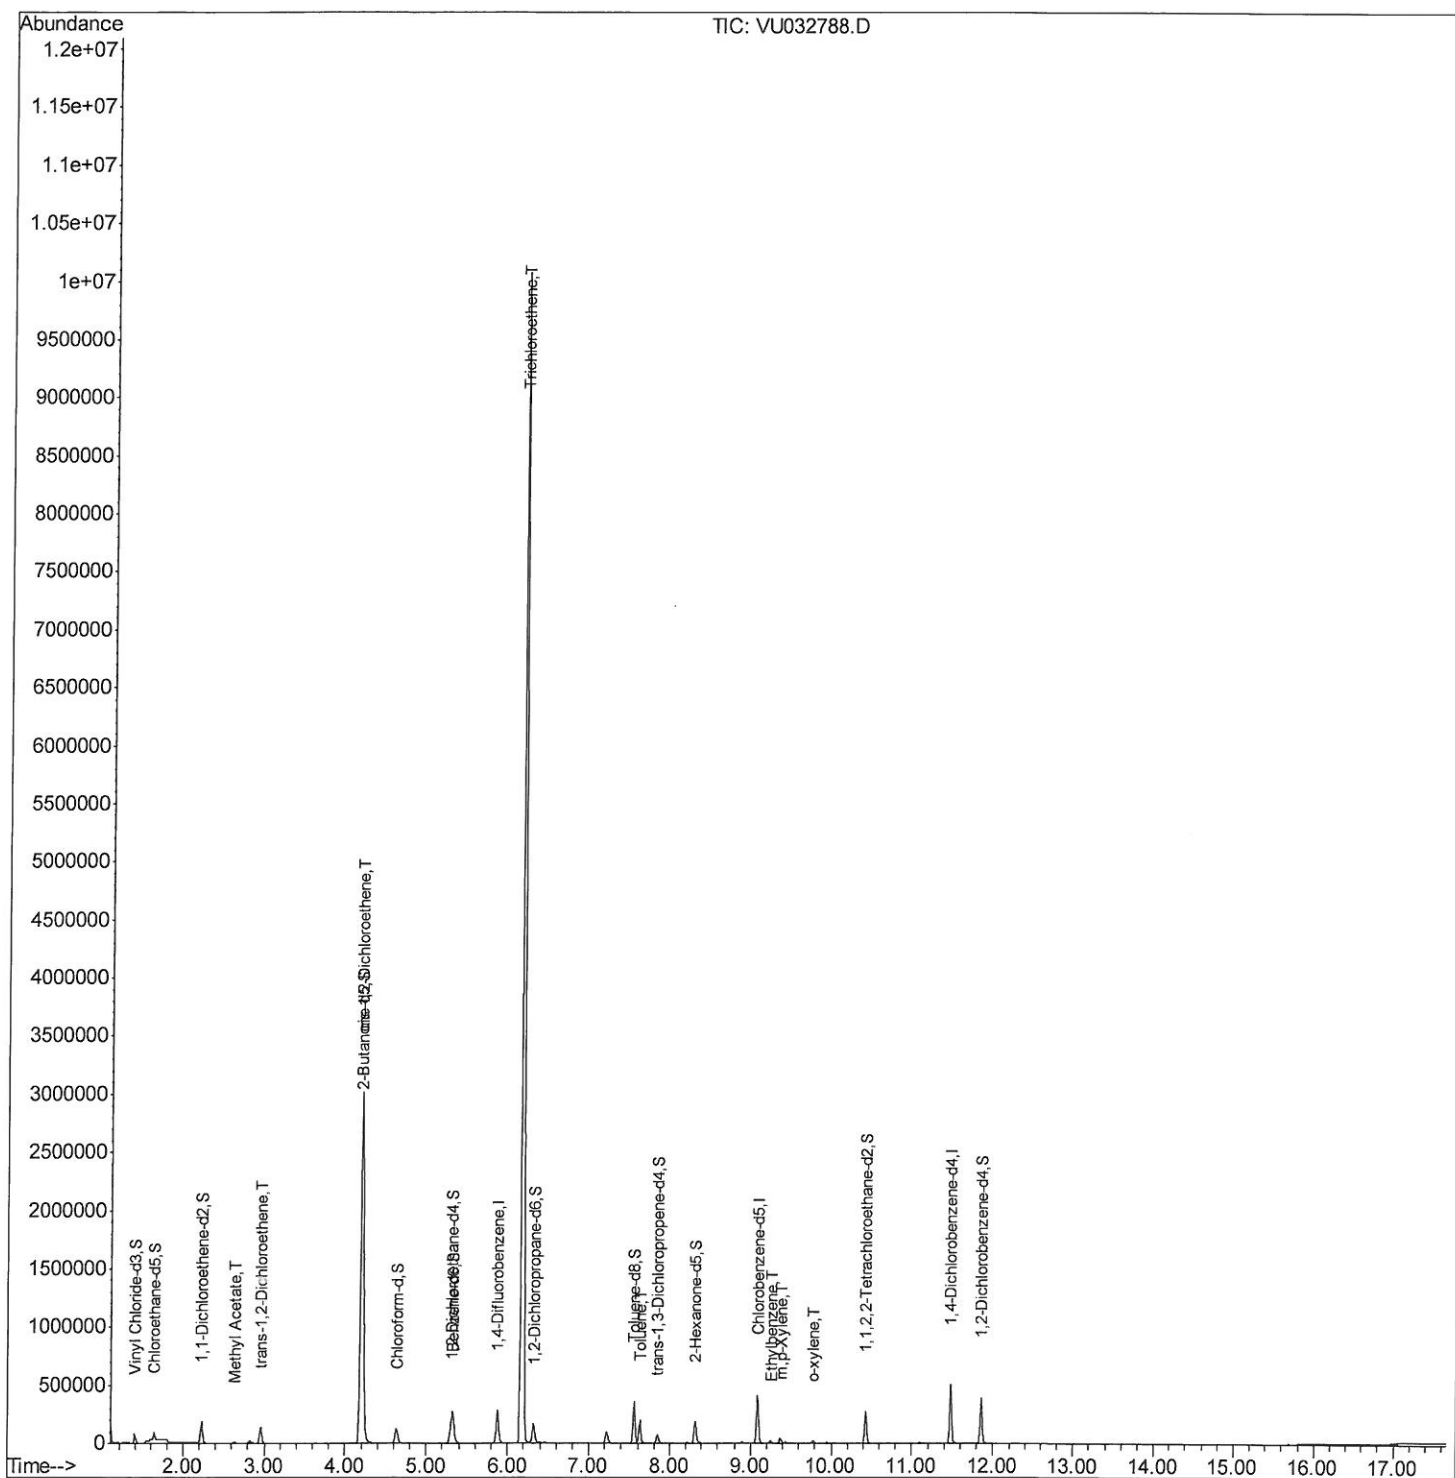

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU061719\
Quantitation Report (Qedit)




Data File : VU032788.D
Acq On : 17 Jun 2019 17:27
Operator : JC/SP
Sample : K3363-07ME
Misc : 3.26g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0JX0ME

Manual Integrations
APPROVED

MMDadoda
6/18/2019 11:28:01 AM

Quant Time: Jun 18 02:43:53 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM061719WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 18 02:39:23 2019
Response via : Initial Calibration

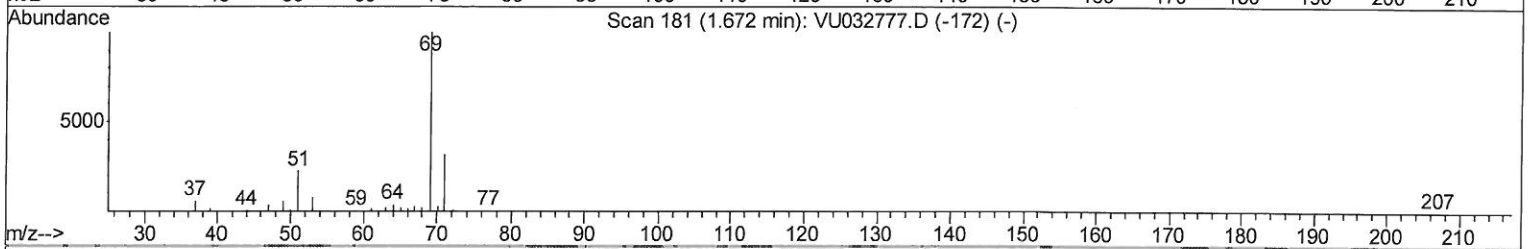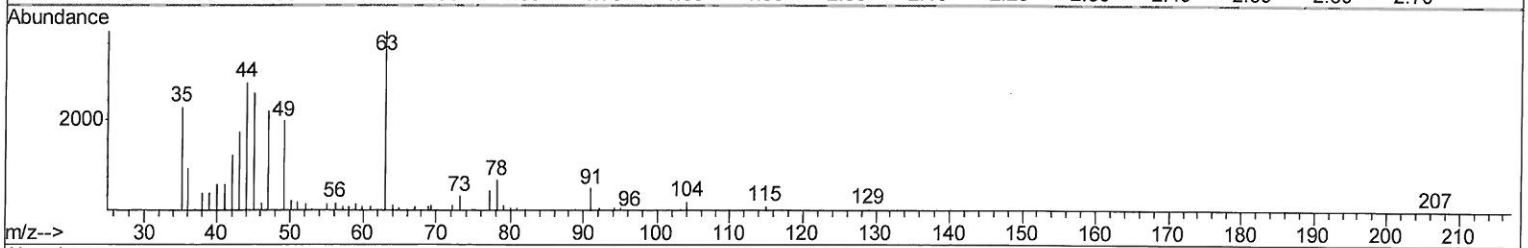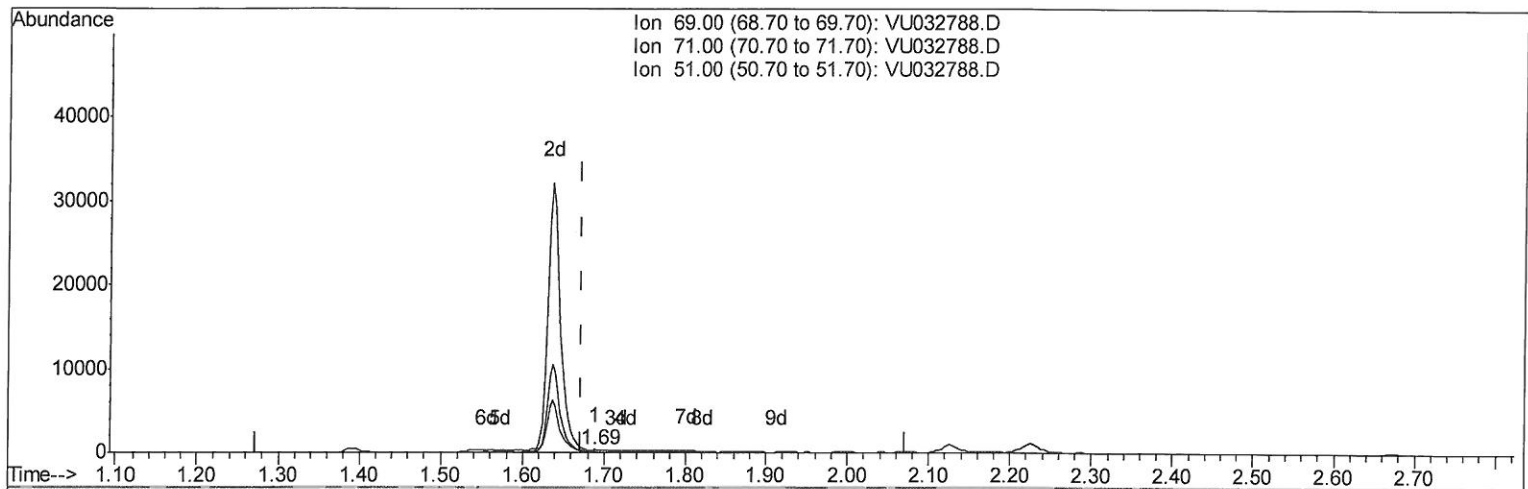

TIC: VU032788.D

(7) Chloroethane-d5 (S)

1.688min (+0.016) 0.12ug/L

response 162

Ion	Exp%	Act%
69.00	100	100
71.00	31.30	0.00#
51.00	30.80	0.00#
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU061719\
Quantitation Report (Qedit)




Data File : VU032788.D
Acq On : 17 Jun 2019 17:27
Operator : JC/SP
Sample : K3363-07ME
Misc : 3.26g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0JX0ME

Manual Integrations
APPROVED

MMDadoda
6/18/2019 11:28:01 AM

Quant Time: Jun 18 02:43:53 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM061719WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 18 02:39:23 2019
Response via : Initial Calibration

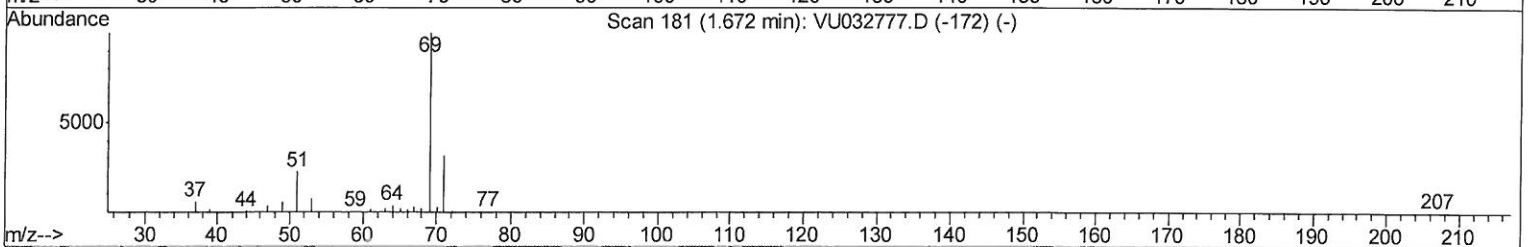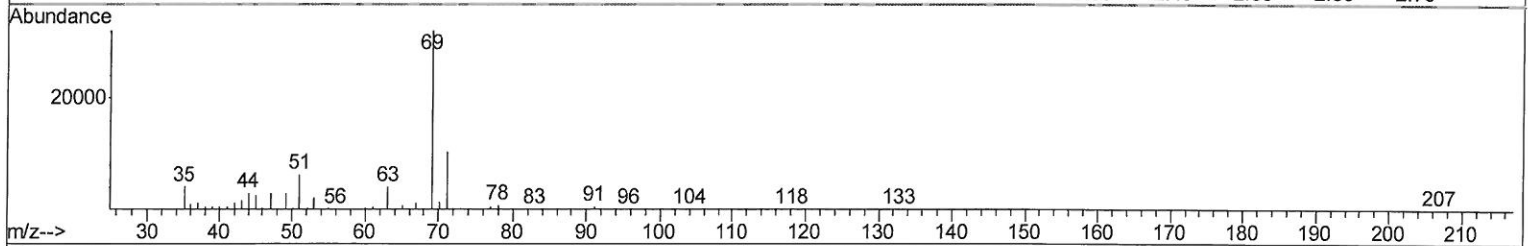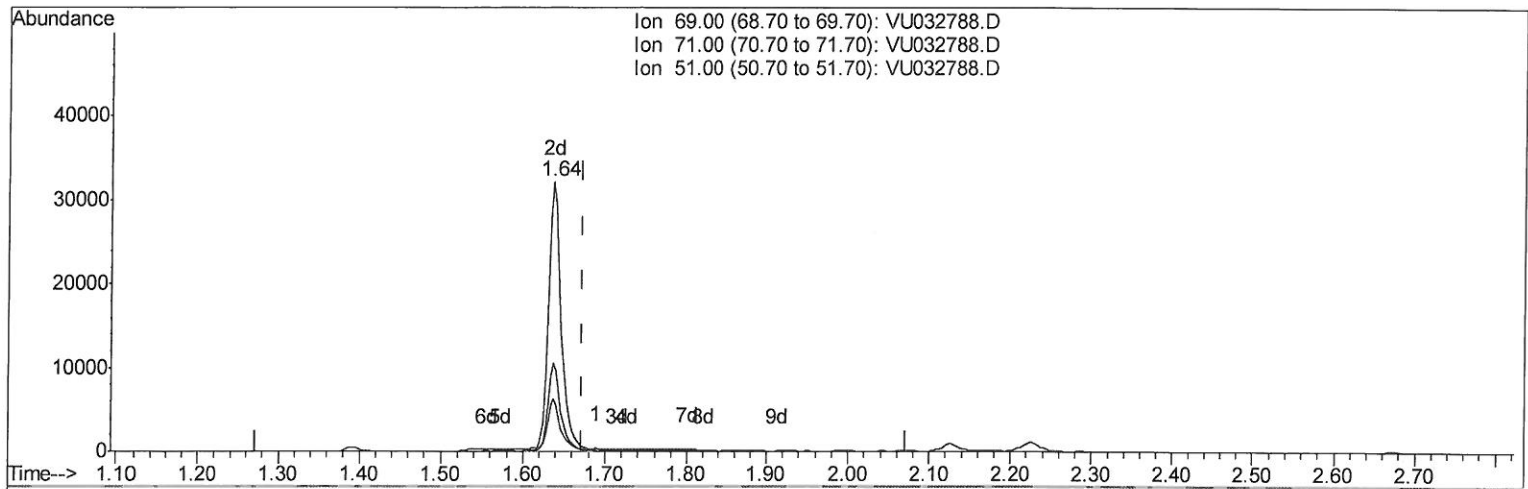

TIC: VU032788.D

(7) Chloroethane-d5 (S)

1.637min (-0.035) 26.88ug/L m

response 35688

Ion	Exp%	Act%
69.00	100	100
71.00	31.30	0.00#
51.00	30.80	0.00#
0.00	0.00	0.00

7MD
6/18/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU061719\
Quantitation Report (Qedit)




Data File : VU032788.D
Acq On : 17 Jun 2019 17:27
Operator : JC/SP
Sample : K3363-07ME
Misc : 3.26g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0JX0ME

Manual Integrations
APPROVED

MMDadoda
6/18/2019 11:28:01 AM

Quant Time: Jun 18 02:43:53 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM061719WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 18 02:39:23 2019
Response via : Initial Calibration

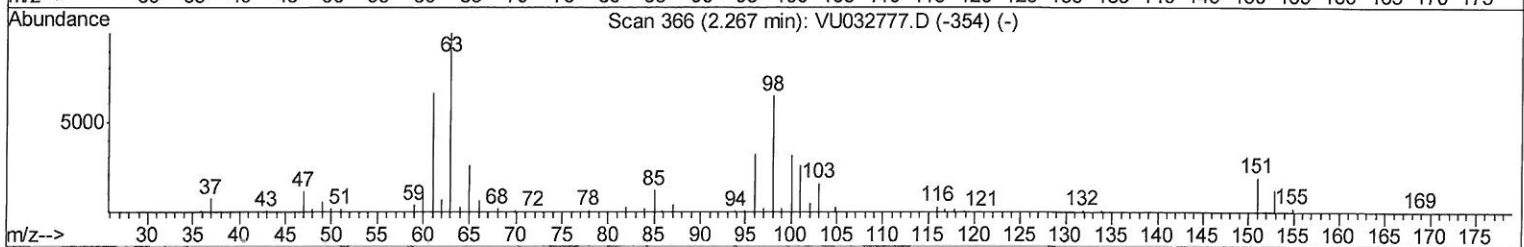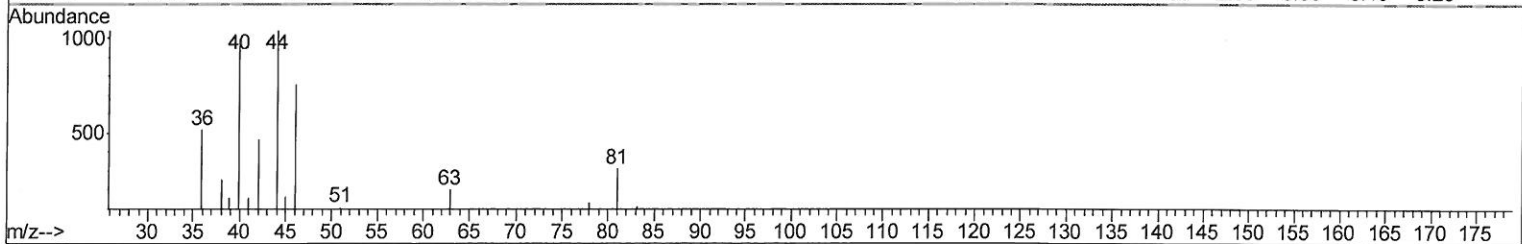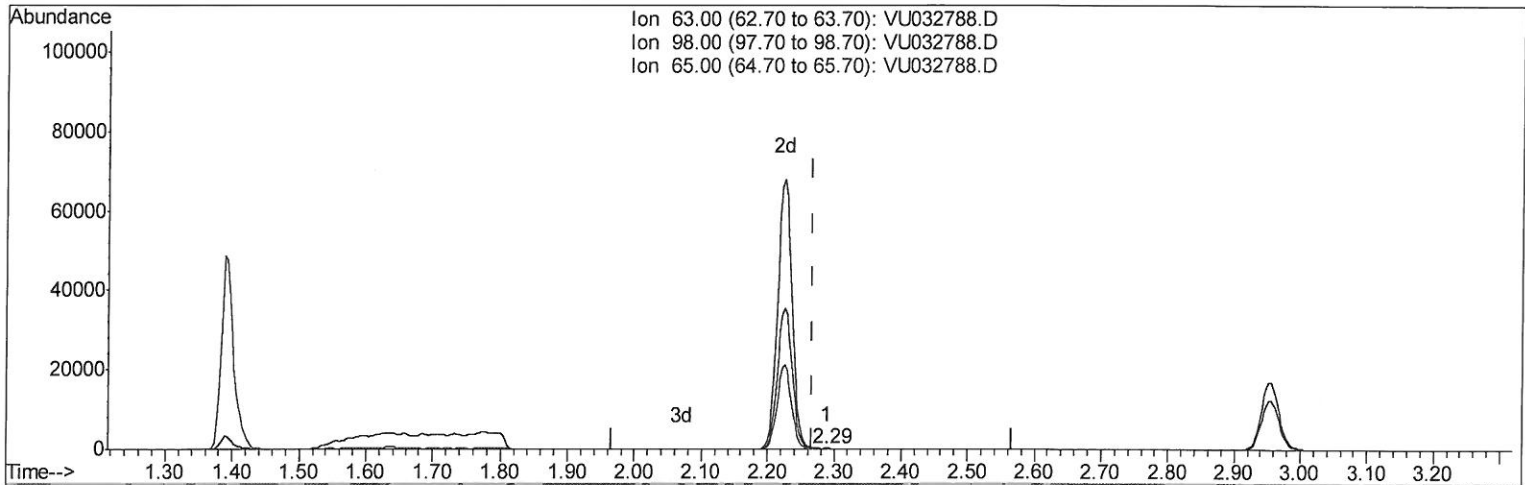

TIC: VU032788.D

(11) 1,1-Dichloroethene-d2 (S)

2.289min (+0.022) 0.04ug/L

response 125

Ion	Exp%	Act%
63.00	100	100
98.00	69.60	0.00#
65.00	23.50	0.00#
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU061719\
Quantitation Report (Qedit)




Data File : VU032788.D
Acq On : 17 Jun 2019 17:27
Operator : JC/SP
Sample : K3363-07ME
Misc : 3.26g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0JX0ME

Manual Integrations
APPROVED

MMDadoda
6/18/2019 11:28:01 AM

Quant Time: Jun 18 02:43:53 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM061719WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 18 02:39:23 2019
Response via : Initial Calibration

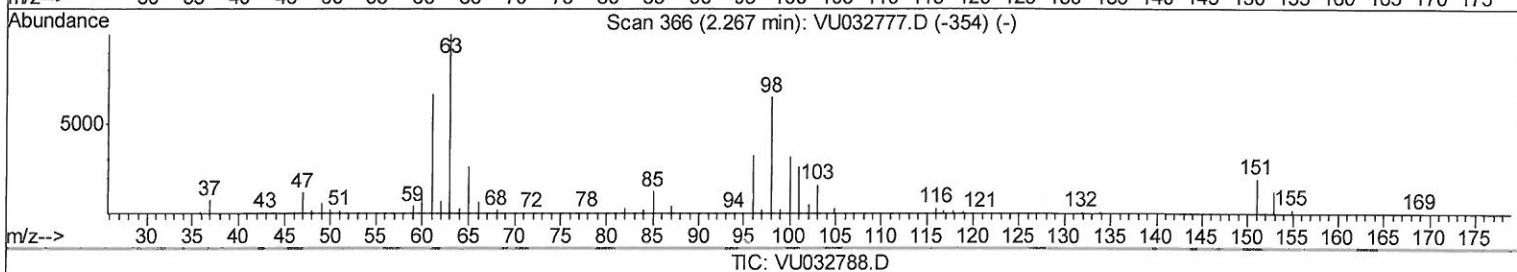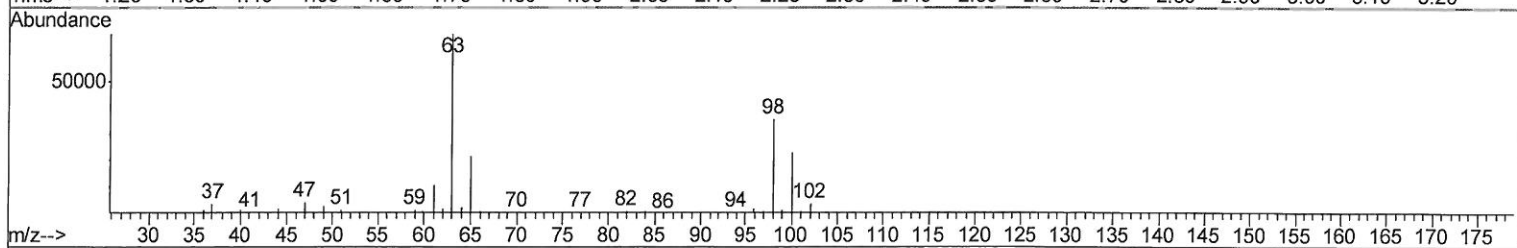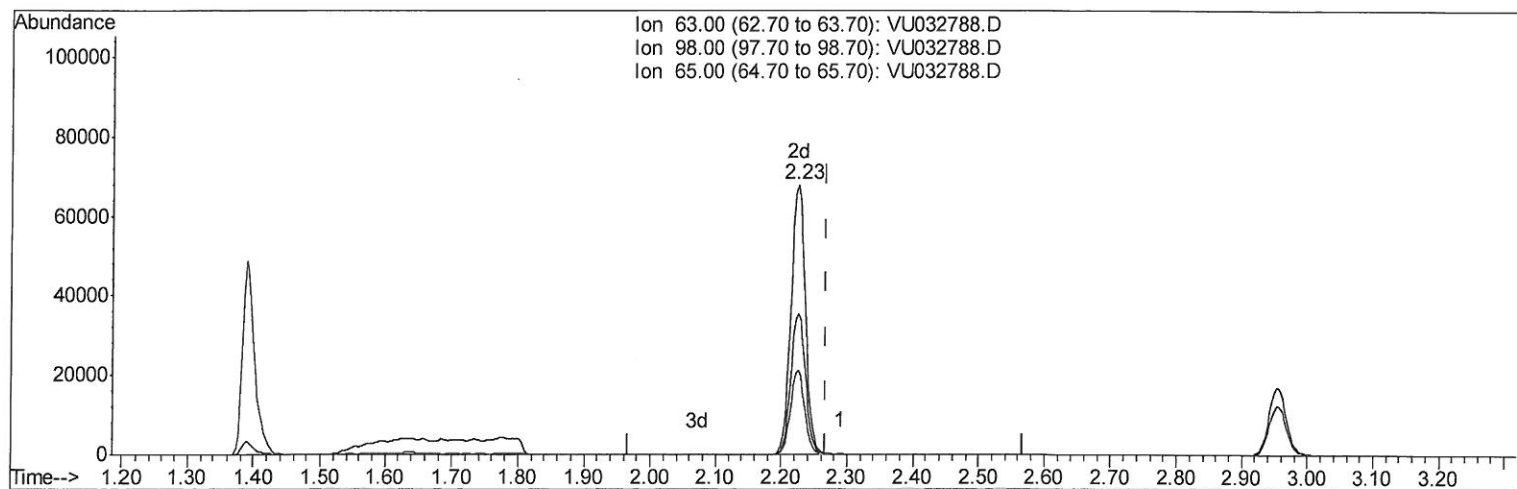

(11) 1,1-Dichloroethene-d2 (S)

2.225min (-0.042) 30.67ug/L m

response 102842

Ion	Exp%	Act%
63.00	100	100
98.00	69.60	0.00#
65.00	23.50	0.00#
0.00	0.00	0.00

7 mg
6/18/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU061719\
Quantitation Report (QT/LSC Reviewed)

Data File : VU032788.D
Acq On : 17 Jun 2019 17:27
Operator : JC/SP
Sample : K3363-07ME
Misc : 3.26g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0JX0ME

Manual Integrations
APPROVED

MMDadoda
6/18/2019 11:28:01 AM

Quant Time: Jun 18 04:19:58 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM061719WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 18 02:39:23 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.87	114	243592	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	235570	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	131063	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	61278	36.81	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	73.62%
7) Chloroethane-d5	1.64	69	35688m	26.88	ug/L	-0.04
Spiked Amount	50.000	Range	70 - 130	Recovery	=	53.76%#
11) 1,1-Dichloroethene-d2	2.23	63	102842m	30.67	ug/L	-0.04
Spiked Amount	50.000	Range	60 - 125	Recovery	=	61.34%
21) 2-Butanone-d5	4.19	46	114948	82.96	ug/L	0.02
Spiked Amount	100.000	Range	40 - 130	Recovery	=	82.96%
24) Chloroform-d	4.64	84	128042	39.56	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	79.12%
26) 1,2-Dichloroethane-d4	5.30	65	89195	41.38	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	82.76%
32) Benzene-d6	5.32	84	254796	41.49	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	82.98%
36) 1,2-Dichloropropane-d6	6.32	67	82068	41.95	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	83.90%
41) Toluene-d8	7.56	98	237800	41.35	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	82.70%
43) trans-1,3-Dichloropropene-	7.85	79	41766	41.04	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	82.08%
47) 2-Hexanone-d5	8.32	63	79912	87.49	ug/L	0.01
Spiked Amount	100.000	Range	45 - 130	Recovery	=	87.49%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	125596	41.53	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	83.06%
64) 1,2-Dichlorobenzene-d4	11.86	152	105448	41.58	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	83.16%

Target Compounds

					Qvalue
15) Methyl Acetate	2.63	43	7548	3.479	ug/L 94
17) trans-1,2-Dichloroethene	2.96	96	49535	29.778	ug/L 99
20) cis-1,2-Dichloroethene	4.21	96	1663895	918.179	ug/L 97
34) Trichloroethene	6.18	95	3356893	1851.396	ug/L 97
42) Toluene	7.63	91	145306	19.790	ug/L 98
52) Ethylbenzene	9.25	91	12246	1.507	ug/L 97
53) m,p-Xylene	9.37	106	12039	3.926	ug/L 97
54) o-xylene	9.78	106	5244	1.751	ug/L 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed