


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU061719\
 Data File : VU032770.D
 Acq On : 17 Jun 2019 08:54
 Operator : JC/SP
 Sample : BFB56
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB56

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM061719WMA.M
 Title : VOC Analysis
 Last Update : Tue Jun 18 02:39:23 2019

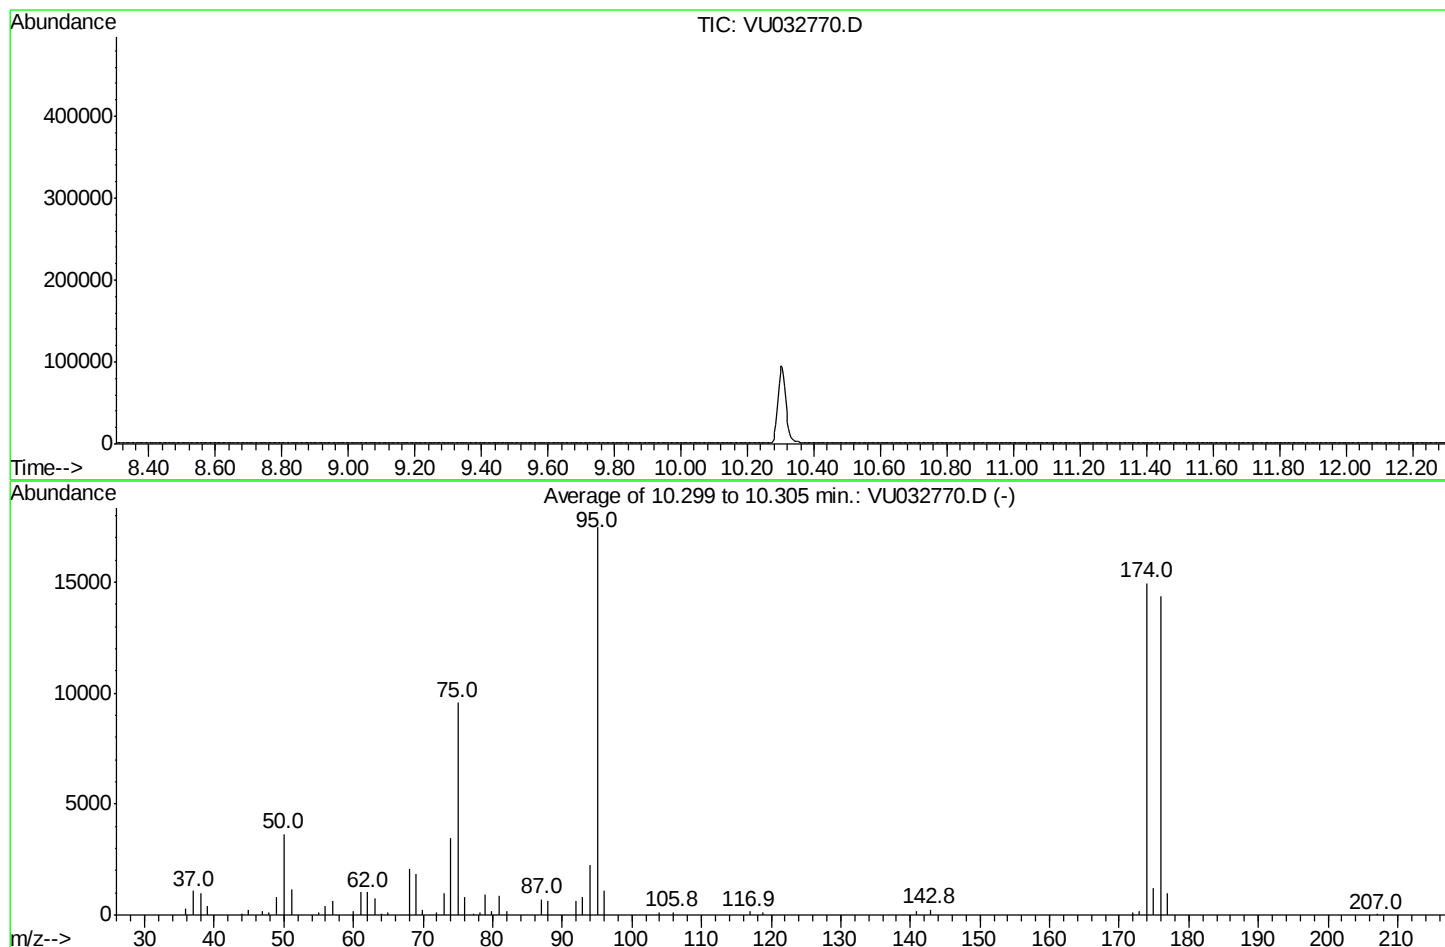

AutoFind: Scans 2864, 2865, 2866; Background Corrected with Scan 2854

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	3642	PASS
75	95	30	80	54.7	9562	PASS
95	95	100	100	100.0	17469	PASS
96	95	5	9	6.3	1094	PASS
173	174	0.00	2	1.3	188	PASS
174	95	50	120	85.5	14942	PASS
175	174	5	9	8.2	1225	PASS
176	174	95	101	96.0	14338	PASS
177	176	5	9	7.0	1004	PASS

Scan 2854 (10.266 min): VU032770.D
BFB56

m/z	Abundance
40.00	825.0
44.00	449.0

Instrument :
MSVOA_U
ClientSampleId :
BFB56

m/z	Abundance
35.90	303.0
37.00	1065.0
38.00	965.0
39.00	439.0
40.00	854.0
43.90	520.0
44.90	232.0
46.90	235.0
47.90	136.0
49.00	733.0
50.00	3553.0
51.10	1211.0
55.10	101.0
56.00	347.0
57.00	598.0
59.90	202.0
61.00	926.0
62.00	1008.0
63.00	767.0
65.00	103.0
68.00	2053.0
69.00	1777.0
69.90	196.0
71.90	127.0
73.00	931.0
74.00	3288.0
75.00	9260.0
76.10	788.0
78.10	134.0
78.90	873.0
79.90	181.0
80.90	820.0
82.00	167.0
87.00	647.0
88.00	651.0
92.00	597.0
93.00	785.0
94.00	2050.0
95.00	16712.0
96.00	1033.0
104.00	121.0
105.90	123.0
116.90	169.0
118.90	116.0
140.80	151.0
142.80	231.0
171.90	118.0
172.90	185.0
174.00	14085.0
174.90	1129.0
176.00	13457.0
177.00	960.0

Instrument :
MSVOA_U
ClientSampleId :
BFB56

m/z	Abundance
36.00	302.0
37.00	1116.0
38.00	1048.0
39.00	430.0
40.00	826.0
43.90	522.0
44.90	231.0
46.90	206.0
47.90	152.0
49.00	809.0
50.00	3766.0
51.00	1205.0
55.00	117.0
56.00	399.0
57.00	618.0
59.90	197.0
61.00	1062.0
62.00	1087.0
63.00	784.0
65.00	116.0
68.00	2120.0
69.00	1920.0
69.90	245.0
71.90	146.0
73.00	1024.0
74.00	3601.0
75.00	9806.0
76.00	851.0
78.10	143.0
78.90	963.0
79.90	178.0
80.90	902.0
82.00	197.0
87.00	734.0
87.90	666.0
92.00	687.0
93.00	802.0
94.00	2353.0
95.00	18080.0
96.10	1103.0
104.00	128.0
105.90	139.0
116.90	189.0
118.80	133.0
140.90	149.0
142.90	254.0
171.90	146.0
172.90	194.0
174.00	15354.0
174.90	1289.0
176.00	14818.0
177.00	1052.0
207.00	102.0

Instrument :
MSVOA_U
ClientSampleId :
BFB56

m/z	Abundance
36.00	264.0
37.00	1082.0
38.00	994.0
39.00	423.0
40.00	786.0
43.90	481.0
44.90	195.0
46.80	159.0
47.90	151.0
49.00	810.0
50.00	3608.0
51.00	1069.0
54.90	112.0
55.90	406.0
57.00	610.0
59.90	168.0
61.00	1075.0
62.00	1018.0
63.00	748.0
64.00	115.0
65.00	114.0
68.00	2027.0
69.00	1908.0
69.90	243.0
71.90	134.0
73.00	952.0
74.00	3474.0
75.00	9622.0
76.00	793.0
77.20	107.0
78.10	130.0
78.90	971.0
79.90	181.0
80.90	888.0
82.00	183.0
87.00	756.0
87.90	615.0
92.00	678.0
92.90	812.0
94.00	2414.0
95.00	17616.0
96.10	1148.0
104.00	105.0
105.80	132.0
116.90	153.0
118.80	147.0
140.90	178.0
142.90	276.0
171.90	160.0
172.90	186.0
174.00	15388.0
174.90	1257.0
176.00	14740.0
177.00	1000.0

Instrument :
MSVOA_U
ClientSampleId :
BFB56