


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061720\
 Data File : VU038935.D
 Acq On : 17 Jun 2020 10:32
 Operator : SY/MD
 Sample : BFB15
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB15

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR061720WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Jun 17 11:08:56 2020

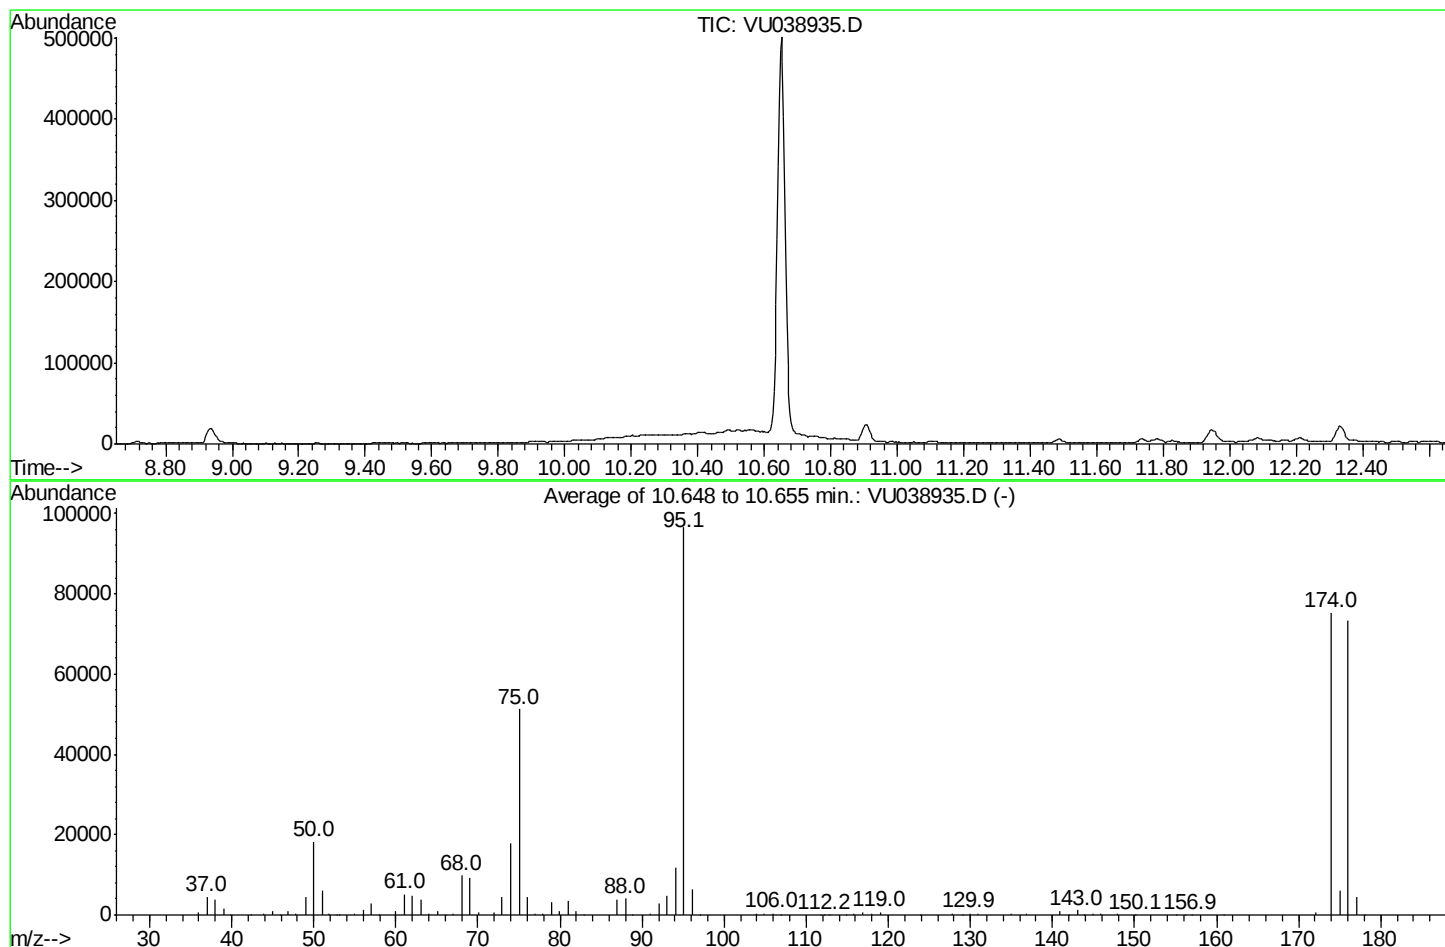

AutoFind: Scans 2895, 2896, 2897; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	18338	PASS
75	95	30	80	53.1	51280	PASS
95	95	100	100	100.0	96539	PASS
96	95	5	9	6.6	6335	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	78.0	75346	PASS
175	174	5	9	7.9	5984	PASS
176	174	95	101	97.3	73333	PASS
177	176	5	9	6.2	4583	PASS

m/z	Abundance
36.00	747.0
37.00	4628.0
38.00	4096.0
39.10	2231.0
39.90	283.0
41.00	783.0
42.00	291.0
43.10	2070.0
44.00	1422.0
44.90	1038.0
46.90	1116.0
47.80	519.0
49.00	4489.0
50.00	19016.0
51.00	6248.0
51.90	327.0
55.00	722.0
56.10	1853.0
57.00	3234.0
58.00	151.0
59.90	977.0
61.00	5074.0
62.00	5051.0
63.00	3948.0
64.00	397.0
65.00	796.0
66.10	198.0
67.00	542.0
68.00	10006.0
69.00	10126.0
70.10	1012.0
71.10	4280.0
72.00	827.0
73.00	4786.0
74.00	18016.0
75.00	51936.0
76.00	4739.0
76.90	644.0
77.90	525.0
79.00	3291.0
79.90	1010.0
81.00	3464.0
81.90	1088.0
83.00	431.0
87.00	3934.0
88.00	3779.0
90.90	422.0
92.00	2978.0
93.00	4778.0
94.10	12018.0
95.10	95752.0
96.10	6286.0
97.00	245.0
103.90	463.0
104.80	134.0
105.90	457.0
106.80	118.0
111.10	390.0
112.20	124.0
114.90	163.0
115.80	338.0
117.00	665.0
118.00	422.0
119.00	725.0
123.90	123.0
127.80	377.0
129.00	158.0
129.90	340.0
130.90	160.0
134.90	192.0
136.90	219.0
140.90	908.0
143.00	1330.0
145.00	268.0
145.80	210.0
147.90	284.0
155.10	219.0
156.20	175.0
156.90	144.0
158.90	234.0
161.00	112.0
172.10	783.0
174.00	74096.0
175.10	5916.0
176.00	71608.0
177.00	4386.0
178.00	145.0

Instrument :
MSVOA_U
ClientSampleId :
BFB15

m/z	Abundance
35.90	775.0
37.00	4564.0
38.00	4147.0
39.10	2068.0
39.90	340.0
41.00	782.0
42.00	220.0
42.30	221.0
43.10	2140.0
44.00	1282.0
45.00	990.0
45.90	110.0
46.90	1134.0
47.80	481.0
49.00	4472.0
50.00	18864.0
51.00	6115.0
51.90	302.0
52.70	131.0
55.00	751.0
56.00	1868.0
57.00	3271.0
57.90	144.0
59.90	994.0
61.10	5411.0
62.00	4968.0
63.00	3904.0
64.10	399.0
65.10	831.0
66.10	137.0
67.00	548.0
68.00	10233.0
69.00	10101.0
70.10	1067.0
71.10	4150.0
72.10	884.0
73.00	4717.0
74.00	18704.0
75.00	52776.0
76.00	4527.0
76.90	619.0
77.90	438.0
78.90	3345.0
80.00	1047.0
81.00	3665.0
81.90	1097.0
82.90	372.0
87.00	4080.0
87.90	4189.0
90.90	412.0
92.00	3130.0
93.00	4768.0
94.10	12399.0
95.10	99808.0
96.10	6489.0
97.00	273.0
103.90	477.0
104.90	186.0
105.90	462.0
106.90	107.0
109.90	101.0
111.10	382.0
111.80	100.0
112.20	124.0
112.80	105.0
115.90	349.0
116.90	693.0
117.90	474.0
119.00	826.0
123.90	138.0
127.80	381.0
129.00	125.0
129.90	421.0
130.90	185.0
134.90	202.0
136.80	194.0
140.90	965.0
142.10	136.0
143.00	1401.0
145.00	216.0
145.80	189.0
148.00	310.0
155.10	296.0
156.20	151.0
157.00	157.0
159.00	254.0
160.90	110.0
172.00	829.0
174.00	77672.0
175.10	6198.0
176.00	75800.0
177.00	4783.0

Instrument :
MSVOA_U
ClientSampleId :
BFB15

178.00195.0

243.30111.0

Instrument :
MSVOA_U
ClientSampleId :
BFB15

m/z	Abundance
35.90	812.0
37.00	4235.0
38.00	3835.0
39.00	1831.0
39.90	371.0
41.00	874.0
42.20	222.0
43.10	2085.0
44.00	1184.0
44.90	868.0
45.90	155.0
46.90	1007.0
47.90	448.0
49.00	4130.0
50.00	17136.0
51.00	5434.0
51.90	306.0
52.70	191.0
53.10	118.0
55.00	783.0
56.00	1734.0
57.00	2876.0
57.90	131.0
59.90	936.0
61.10	5099.0
62.00	4376.0
63.10	3740.0
64.10	378.0
65.10	825.0
67.00	468.0
68.00	9343.0
69.00	9396.0
70.10	1040.0
71.10	4162.0
72.10	749.0
73.00	4325.0
74.00	17312.0
75.00	49128.0
76.00	3952.0
76.90	564.0
77.80	356.0
78.90	3289.0
80.00	1014.0
81.00	3249.0
81.90	926.0
82.90	272.0
87.00	3894.0
87.90	4028.0
88.80	145.0
91.00	383.0
92.00	2868.0
93.00	4528.0
94.10	11263.0
95.10	94360.0
96.10	6230.0
97.00	320.0
103.90	431.0
105.00	211.0
106.00	481.0
109.90	106.0
111.10	379.0
112.90	115.0
115.90	377.0
116.90	690.0
117.90	408.0
119.00	779.0
123.90	122.0
127.80	384.0
129.90	443.0
130.80	191.0
134.90	168.0
136.80	186.0
141.00	941.0
142.00	102.0
143.00	1279.0
143.90	102.0
145.00	177.0
145.90	141.0
148.00	293.0
150.10	114.0
155.10	373.0
157.00	126.0
159.10	306.0
160.80	124.0
172.00	764.0
174.00	74272.0
175.10	5840.0
176.00	72592.0
177.00	4581.0
178.00	167.0
243.30	134.0

Instrument :
MSVOA_U
ClientSampleId :
BFB15

m/z	Abundance
38.10	203.0
39.10	351.0
39.90	301.0
41.00	873.0
41.90	223.0
43.00	2136.0
43.90	1022.0
55.00	416.0
56.10	448.0
57.10	103.0
67.00	137.0
69.10	476.0
70.00	274.0
71.00	5495.0
72.00	256.0
72.90	137.0
77.00	126.0
83.00	288.0
95.10	101.0
97.10	124.0
98.00	138.0
110.10	219.0
111.00	460.0
143.10	109.0
155.00	208.0
159.10	373.0
173.10	103.0
243.20	132.0

Instrument :
MSVOA_U
ClientSampleId :
BFB15